

Operating Instruction

SS2100i-2 TDLAS Gas Analyzer

ATEX/IECEx: Zone 1



TABLE OF CONTENTS

1: Introduction

How to Use This Manual	1-1
Who should read this manual	1-1
Conventions used in this manual	1-1
General Warnings and Cautions	1-1
Safety warning label	1-2
Equipment labels	1-2
Instructional symbols	1-3
Manufacturer Address	1-4
About the Gas Analyzers	1-4
Sample conditioning system	1-4
Determining firmware version	1-4
How the Analyzers Work	1-5
Differential TDLAS	1-7
Wavelength Modulation Spectroscopy (WMS) Signal Detection	1-7
Getting Familiar with the Analyzer	1-9
Special Safety Symbols Used on the Equipment	1-16

2: Safety

Potential Risks Affecting Personnel	2-1
Mitigating risks	2-1
Explosion hazard	2-2

3: Installation

What Should be Included in the Shipping Box	3-1
Lifting/Carrying the Analyzer	3-1
Inspecting the Analyzer	3-1
Hardware and Tools for Installation	3-2
Hardware	3-2
Tools	3-2
Mounting the Analyzer	3-3
Protective Chassis Ground Connections	3-3
Opening the Analyzer Enclosure Covers	3-4
Cable Installation	3-4
Terminations	3-4
Cable Glands	3-5
Connecting the Solenoid Valves	3-5
Application of Gland Lubricant	3-11
Connecting the Signals and Alarms	3-12
Configuring the RS-232/RS-485 Converter	3-16
Connecting Electrical Power to the Analyzer	3-16
Connecting the Gas Lines	3-19
Changing the 4 to 20 mA Current Loop Mode	3-20

Appendix A: Specifications

Exd Accessory Conditions of Use	A-2
---	-----

Appendix B: Maintenance & Troubleshooting

Gas Leaks	B-1
Excessive Sampling Gas Temperatures and Pressures	B-2
Electrical Noise	B-2

Contamination	B-2
Mirror contamination	B-3
Cleaning the Mirrors	B-3
Tools and supplies	B-3
Determining the type of cell mirror	B-4
Replacing the pressure sensor on a 8 m/28 m cell	B-9
Tools and supplies	B-9
Replacing the pressure sensor on a 0.8 m cell	B-15
Tools and supplies	B-15
Flame Arrestor Replacement and Safety	B-20
Tools Required	B-20
Potential health effects	B-22
Transport Information	B-23
Regulatory Information	B-23
Other information	B-24
Peak Tracking Reset Procedure	B-24
Instrument Issues	B-24
Service Contact	B-30
Service Repair Order	B-30
Packing, Shipping and Storage	B-30
Storage	B-31
Disclaimers	B-31
Warranty	B-31

Appendix C: Analyzer Parts

Analyzer Parts	C-1
--------------------------	-----

Appendix D: Wiring Diagrams

Wiring Diagrams	D-1
---------------------------	-----

1 - INTRODUCTION

Endress+Hauser SS2100i-2 products use SpectraSensors TDLAS technology and are high-speed, diode-laser based extractive analyzers designed for extremely reliable monitoring of very low (trace) to standard concentrations of specific components in various background gases. In order to ensure that the analyzer performs as specified, it is important to closely review the sections of this manual. This manual contains a comprehensive overview of the SS2100i-2 analyzer and step-by-step instructions for:

- Inspecting the analyzer
- Mounting and installing the analyzer
- Troubleshooting the system

How to Use This Manual


Take a moment to familiarize yourself with this manual by reading the "**Table of Contents**".

There are a number of options and "**Table of Contents**" accessories available for the SS2100i-2 analyzers. This manual has been written to address the most common options and accessories. Images, tables and charts have been included to provide a visual understanding of the analyzer and its functions. Special symbols are also used to provide the user with key information regarding the system configuration and/or operation. Pay close attention to this information.

Who should read this manual

This manual should be read and referenced by anyone installing, operating or having direct contact with the analyzer.

Conventions used in this manual

In addition to the symbols and instructional information, this manual is created with "hot links" to enable the user to quickly navigate between different sections within the manual. These links include table, figure and section references and are identified by a pointing finger cursor  when rolling over the text. Simply click on the link to navigate to the associated reference.

General Warnings and Cautions

Instructional icons are provided in this manual and on the SS2200i-2 unit to alert the user of potential hazards, important information and valuable tips. Following are the symbols and associated warning and caution types to observe when servicing the analyzer. Some of these symbols are provided for instructional purposes only and are not labeled on the system.

Safety warning label

The warning label shown below will be affixed to the front side of all analyzer enclosures that contain sample gas.



Hazards may vary by stream composition. One or more of the following conditions may apply.



Flammable. Gases used in the processing of this analyzer may be extremely flammable. Any work in a hazardous area must be carefully controlled to avoid creating any possible ignition sources (e.g., heat, arcing, sparking, etc.).



Toxins. Endress+Hauser analyzers measure a variety of gases, including high-level H_2S . Follow all safety protocols governing toxic gases and potential leaks.



Inhalation. Inhaling toxic gases or fumes may cause physical damage or death.



Technicians are expected to follow all safety protocols established by the customer that are necessary for servicing or operating the analyzer. This may include, but is not limited to, lockout/tag-out procedures, toxic gas monitoring protocols, PPE requirements, hot work permits and other precautions that address safety concerns related to performing service or operation on process equipment located in hazardous areas.

Equipment labels



Warning statement for **hazardous voltage**. Contact may cause electric shock or burn. Turn off and lock out system before servicing.



Failure to follow all directions may result in damage or malfunction of the analyzer.



Maximum voltage and current specifications for the fuse closest to label.



PROTECTIVE EARTH GROUND - Symbol indicates the connection point of the ground wire from the main power source.



FUNCTIONAL EARTH GROUND - Symbol indicates grounding points intended primarily for troubleshooting.

CAUTION

CLASS 3B INVISIBLE LASER
RADIATION WHEN OPEN
AVOID EXPOSURE TO THE BEAM

INVISIBLE LASER RADIATION - Avoid exposure to beam. Class 3b Radiation Product. Refer servicing to the manufacturer or qualified personnel.



Removing label from measurement cell optical head will void analyzer warranty.

Instructional symbols



General notes and important information concerning the installation and operation of the analyzer.



Failure to follow all directions may result in fire.



INVISIBLE LASER RADIATION - Avoid exposure to beam.
Class 3b Radiation Product. Refer servicing to the manufacturer-qualified personnel.



Maximum voltage and current specifications for fuses.

Manufacturer Address

Endress+Hauser
11027 Arrow Route
Rancho Cucamonga, CA 91730
United States
www.endress.com

About the Gas Analyzers

Endress+Hauser analyzers are tunable diode laser (TDL) absorption spectrometers operating in the near- to short-wavelength infrared. Each compact sensor consists of a TDL light source, sample cell and detector specifically configured to enable high sensitivity measurement of a particular component within the presences of other gas phase constituents in the stream. The sensor is controlled by microprocessor-based electronics with embedded software that incorporates advanced operational and data processing algorithms.

Sample conditioning system

The analyzer may be integrated with a sample conditioning system (SCS) that is specifically designed to meet the sample condition requirements for the analyzer while preserving sample integrity and minimizing sample lag time. Refer to the SCS Operating Instruction for more information.

Determining firmware version

When the analyzer is powered on for the first time, the firmware version will display on the system LCD for approximately seven seconds. Refer to "**Powering Up the Analyzer**" in the Description of Device Parameters for this analyzer for operational instructions. The firmware version for each analyzer is also listed on the analyzer calibration certificate.

How the Analyzers Work

The SS2100i-2 analyzers employ tunable diode laser absorption spectroscopy (TDLAS) to measure the concentration of single compounds in gas mixtures. In its simplest form, a tunable diode laser absorption spectrometer typically consists of a sample cell with a mirror at one end, and a mirror or window at the opposite end, through which the laser beam can pass. Refer to Figure 1–1 on page 1–5. The laser beam enters the cell and reflects off the mirror(s) making one or more trips through the sample gas and eventually exiting the cell where the remaining beam intensity is measured by a detector. With the SS2100i-2 analyzers, sample gas flows continuously through the sample cell ensuring that the sample is always representative of the flow in the main pipe.

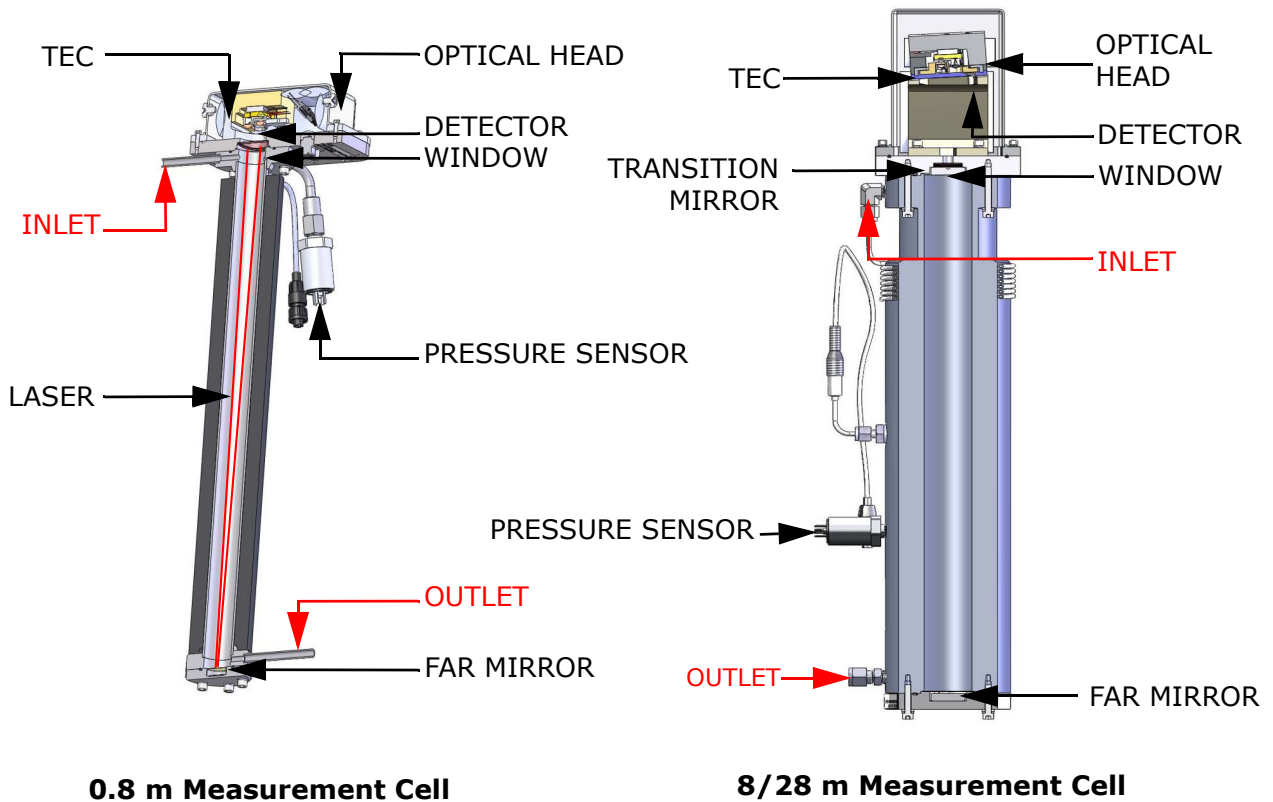


Figure 1–1 Schematic of a typical tunable diode laser absorption spectrometer

Due to their inherent structure, the molecules in the sample gas each have characteristic natural frequencies (or resonances). When the output of the laser is tuned to one of those natural frequencies, the molecules with that particular resonance will absorb energy from the incident beam. That is, as the beam of incident intensity, $I_0(\lambda)$, passes through the sample, attenuation occurs via absorption by the trace gas with absorption cross section $\sigma(\lambda)$. According to the Beer-Lambert absorption law, the intensity remaining, $I(\lambda)$, as measured

by the detector at the end of the beam path of length l (cell length \times number of passes), is given by $I(\lambda) = I_0(\lambda)\exp[-\sigma(\lambda)lN]$, where N represents the species concentration. Thus, the ratio of the absorption measured when the laser is tuned on-resonance versus off-resonance is directly proportional to the number of molecules of that particular species in the beam path, or

$$N = \frac{-1}{\sigma(\lambda)l} \ln \left[\frac{I(\lambda)}{I_0(\lambda)} \right]. \quad (1)$$

Figure 1–2 on page 1–6 shows the typical raw data (in arbitrary units [a.u.]) from a laser absorption spectrometer scan including the incident laser intensity, $I_0(\lambda)$, and the transmitted intensity, $I(\lambda)$, for a clean system and one with contaminated mirrors (shown to illustrate the system's relative intensity to mirror contamination).

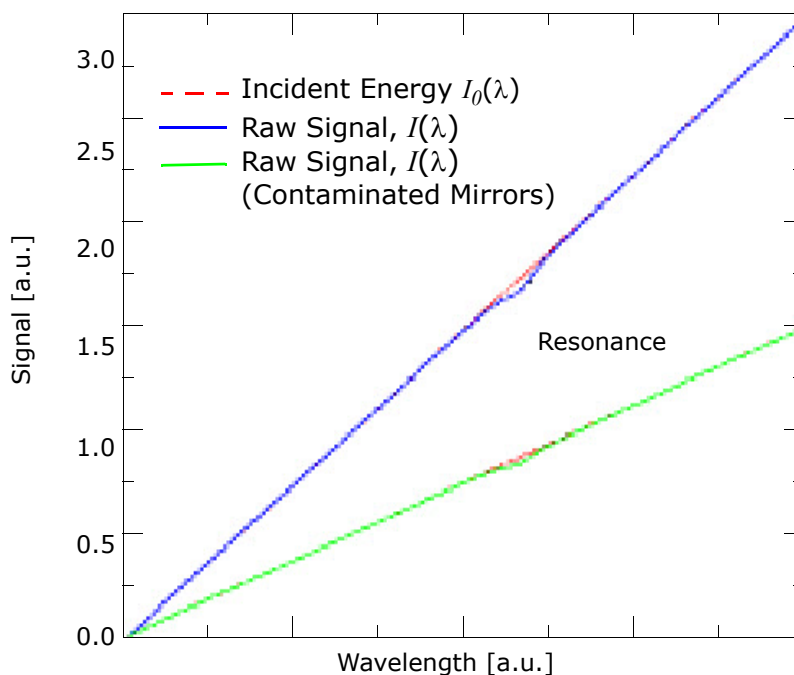


Figure 1–2 Typical raw signal from a tunable diode laser absorption spectrometer with and without mirror contamination

The positive slope of raw data results from ramping the current to tune the laser, which not only increases the wavelength with current, but also causes the corresponding output power to increase. By normalizing the signal by the incident intensity, any laser output fluctuations are canceled, and a typical, yet more pronounced, absorption profile results. Refer to Figure 1–3 on page 1–7.

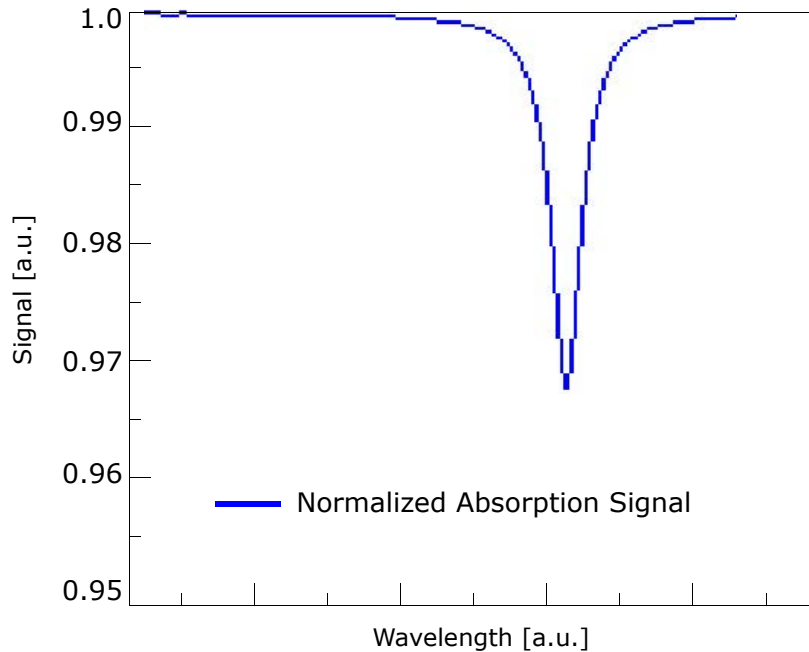


Figure 1-3 Typical normalized absorption signal from a tunable diode laser absorption spectrometer

Note that contamination of the mirrors results solely in lower overall signal. However, by tuning the laser off-resonance as well as on-resonance and normalizing the data, the technique self calibrates every scan resulting in measurements that are unaffected by mirror contamination.

Differential TDLAS

Similar to TDLAS, this Endress+Hauser technology involves subtracting two spectrums from one another. A “dry” spectrum, a response from the sample when the analyte of interest has been completely removed, is subtracted from the “wet” spectrum, a response from the sample when the analyte is present. The remainder is a spectrum of the pure analyte. This technology is used for very low or trace measurements and is also useful when the background matrix changes over time.

Wavelength Modulation Spectroscopy (WMS) Signal Detection

Endress+Hauser takes the fundamental absorption spectroscopy concept a step further by using a sophisticated signal detection technique called wavelength modulation spectroscopy (WMS). When employing WMS, the laser drive current is modulated with a kHz sine wave as the laser is rapidly tuned. A lock-in amplifier is then used to detect the harmonic component of the signal

that is at twice the modulation frequency ($2f$). Refer to Figure 1–4 below, which is shown in arbitrary units (a.u.). This phase-sensitive detection enables the filtering of low-frequency noise caused by turbulence in the sample gas, temperature and/or pressure fluctuations, low-frequency noise in the laser beam or thermal noise in the detector.

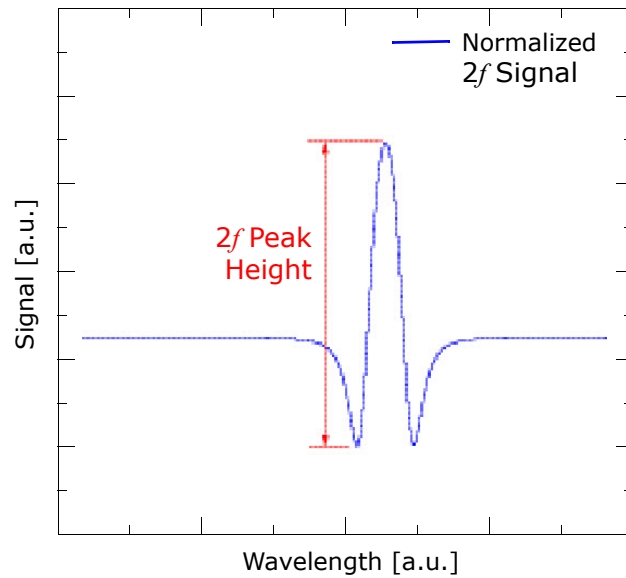


Figure 1–4 Typical normalized $2f$ signal

With the resulting low-noise signal and use of fast post-processing algorithms, reliable parts per million (ppm) or parts per billion (ppb) detection levels are possible (depending on target and background species) at real-time response rates.

All Endress+Hauser TDL gas analyzers employ the same design and hardware platform. Measuring different trace gases in various mixed hydrocarbon background streams is accomplished by selecting a different optimum diode laser wavelength between 700-3000 nm, which provides the least amount of sensitivity to background stream variations.

Getting Familiar with the Analyzer

The analyzer consists of two connected enclosures in a standard cable-coupled configuration, as shown in Figure 1-5 below and Figure 1-6 on page 1-10.

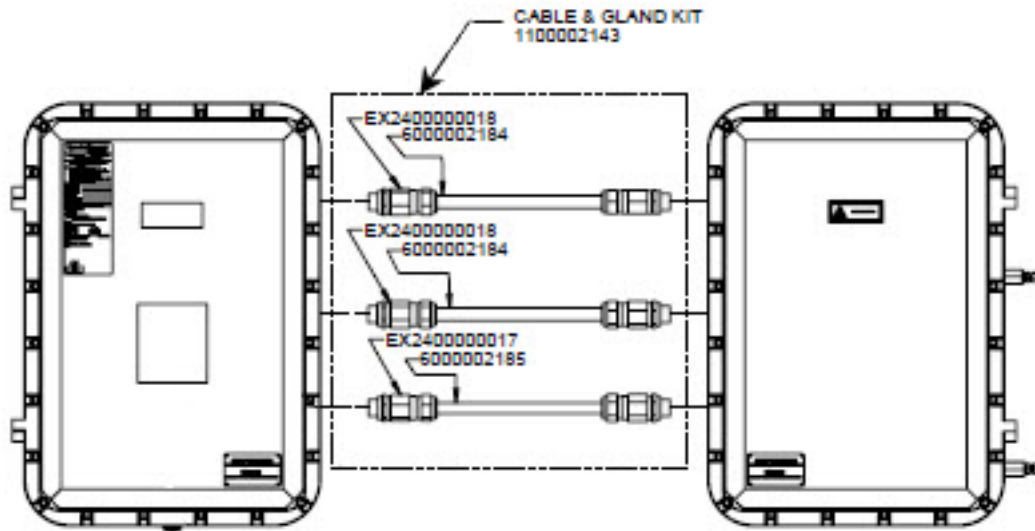


Figure 1-5 Cable-coupled analyzer configuration

The left enclosure (electronics enclosure) contains the control electronics and input/output electrical connections, as shown in Figure 1-7 on page 1-11. The right enclosure (sample cell enclosure) contains the sample cell and heater, as shown in Figure 1-8 on page 1-12 (8/28 m sample cell), Figure 1-9 on page 1-13 (0.8 m sample cell) or Figure 1-10 on page 1-14 (0.1 m sample cell). The keypad and LCD display on the cover of the electronics enclosure are the user interface to the analyzer. Power and signal connections are made via access ports on the bottom of the electronics enclosure. Tube fittings on the right side of the sample cell enclosure are for sample supply and return connections. Both enclosures are mounted on a Unistrut® frame.

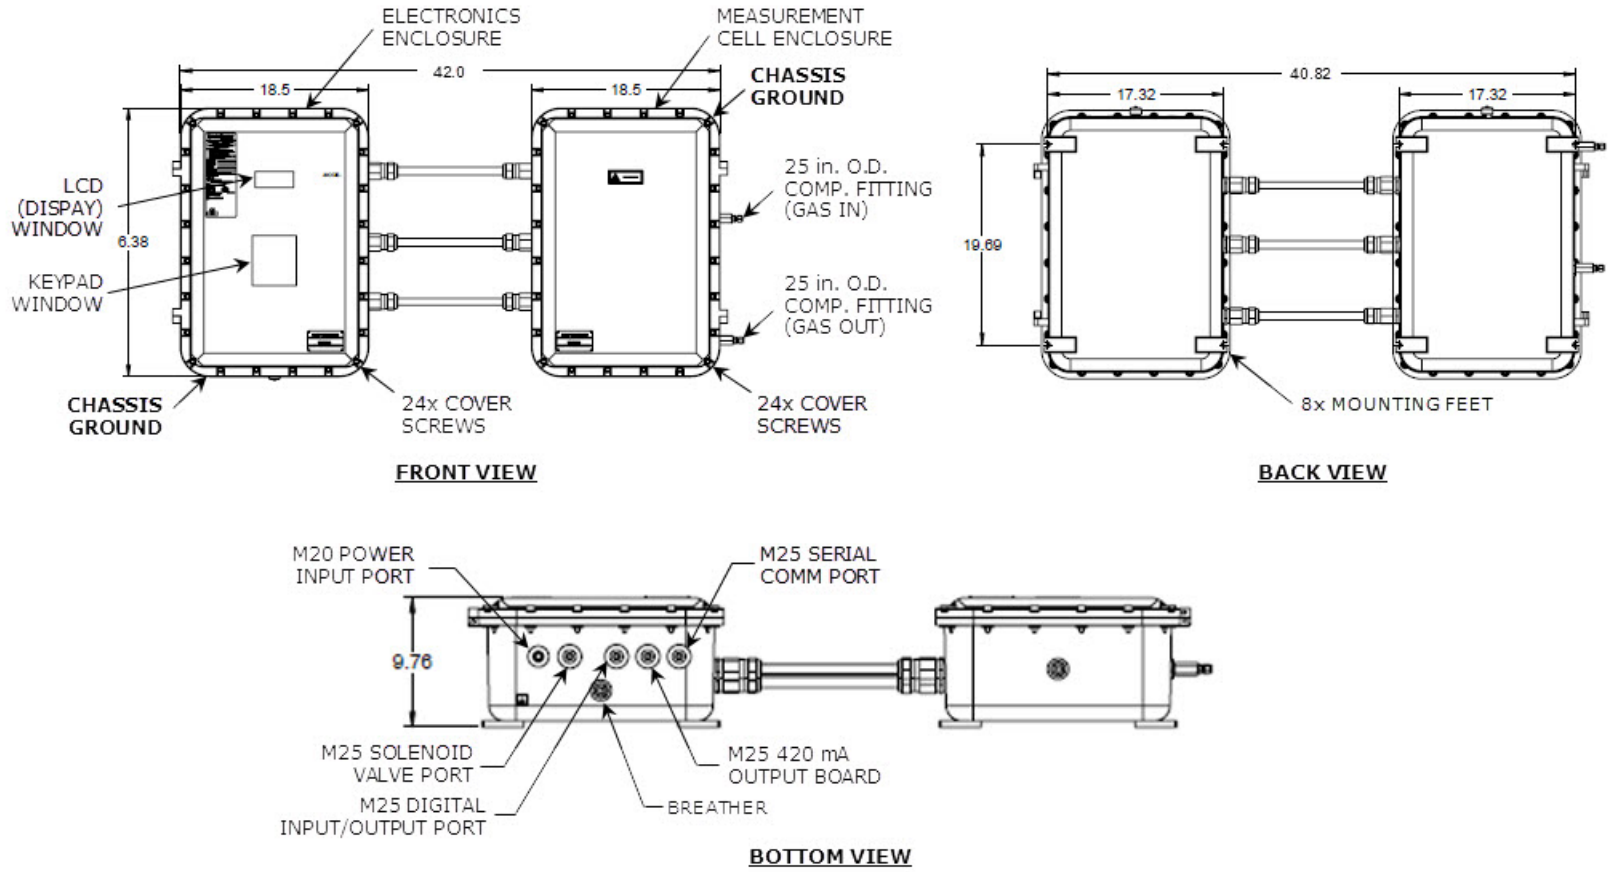


Figure 1-6 Dimensions and Mounting for Electronics and sample cell enclosures (cable-coupled configuration)

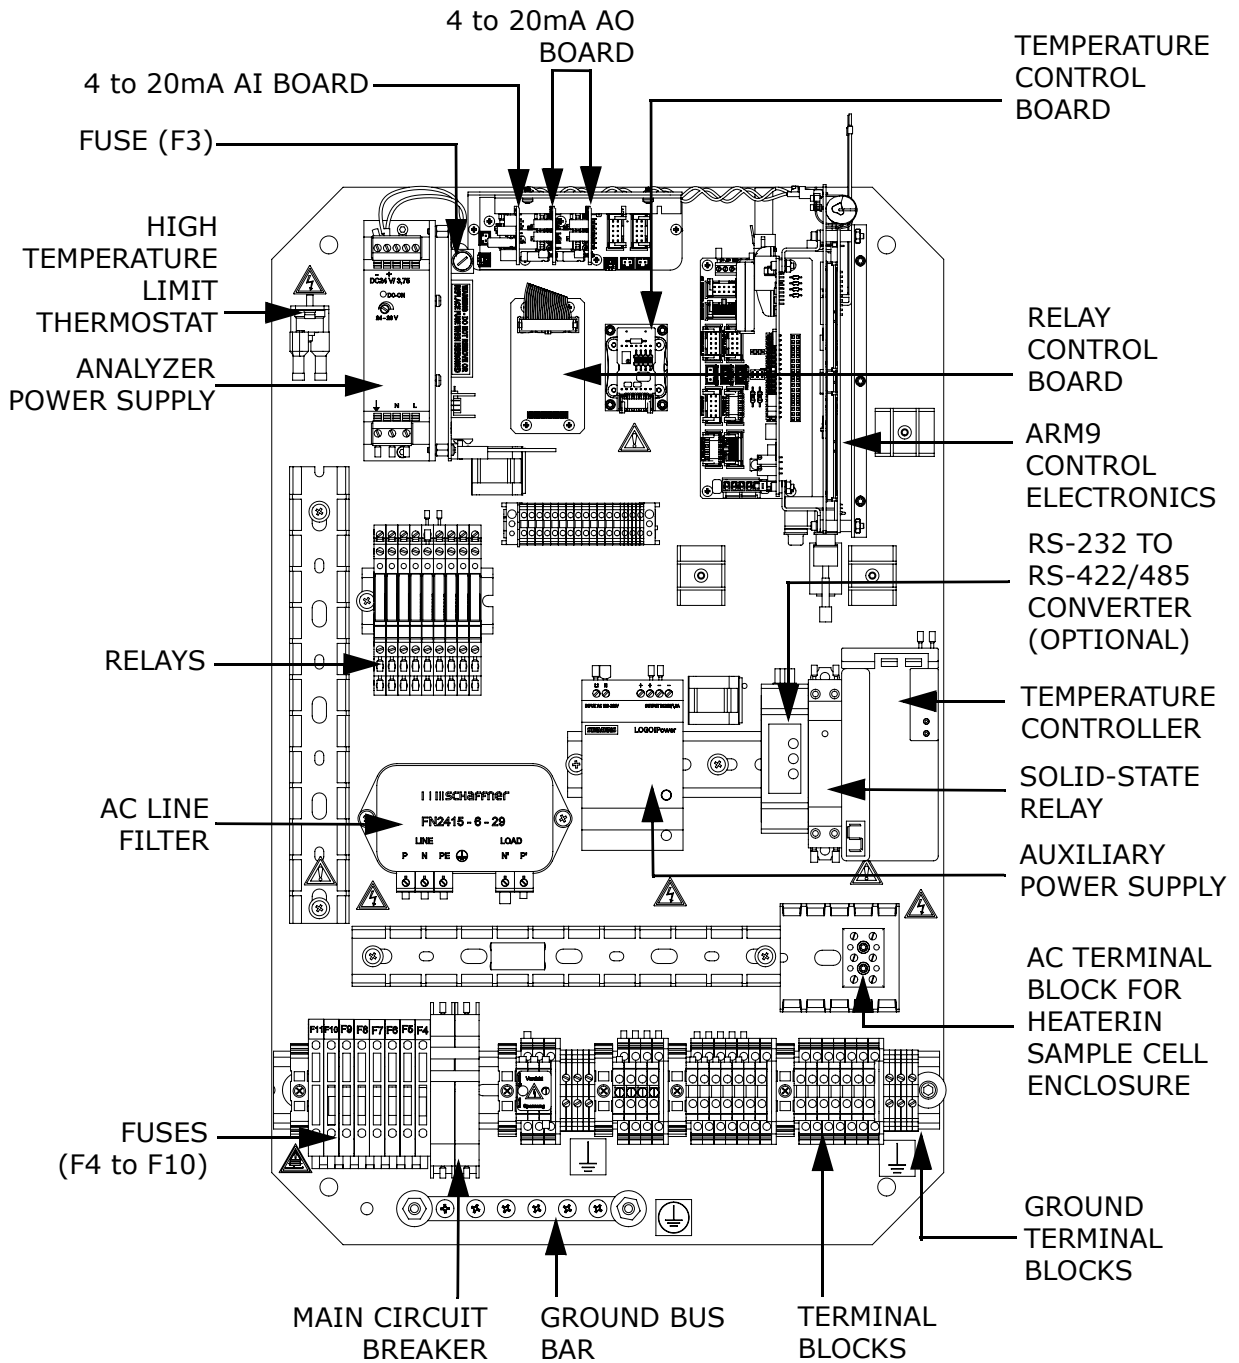


Figure 1-7 Components in electronics enclosure

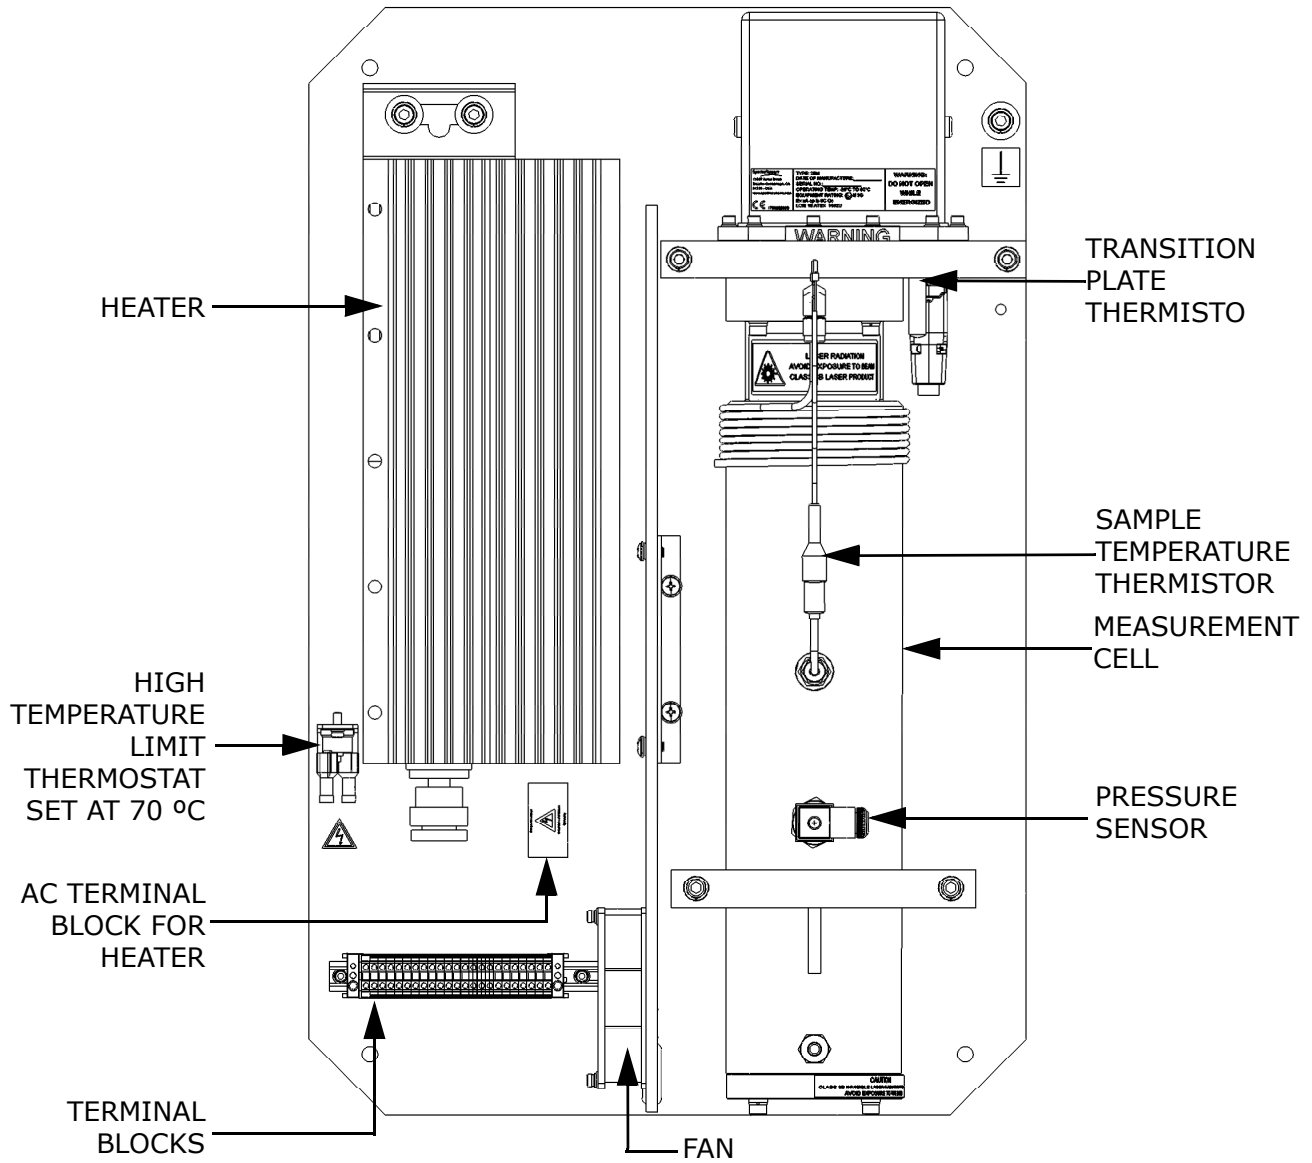


Figure 1-8 Components in 8/28 m sample cell enclosure

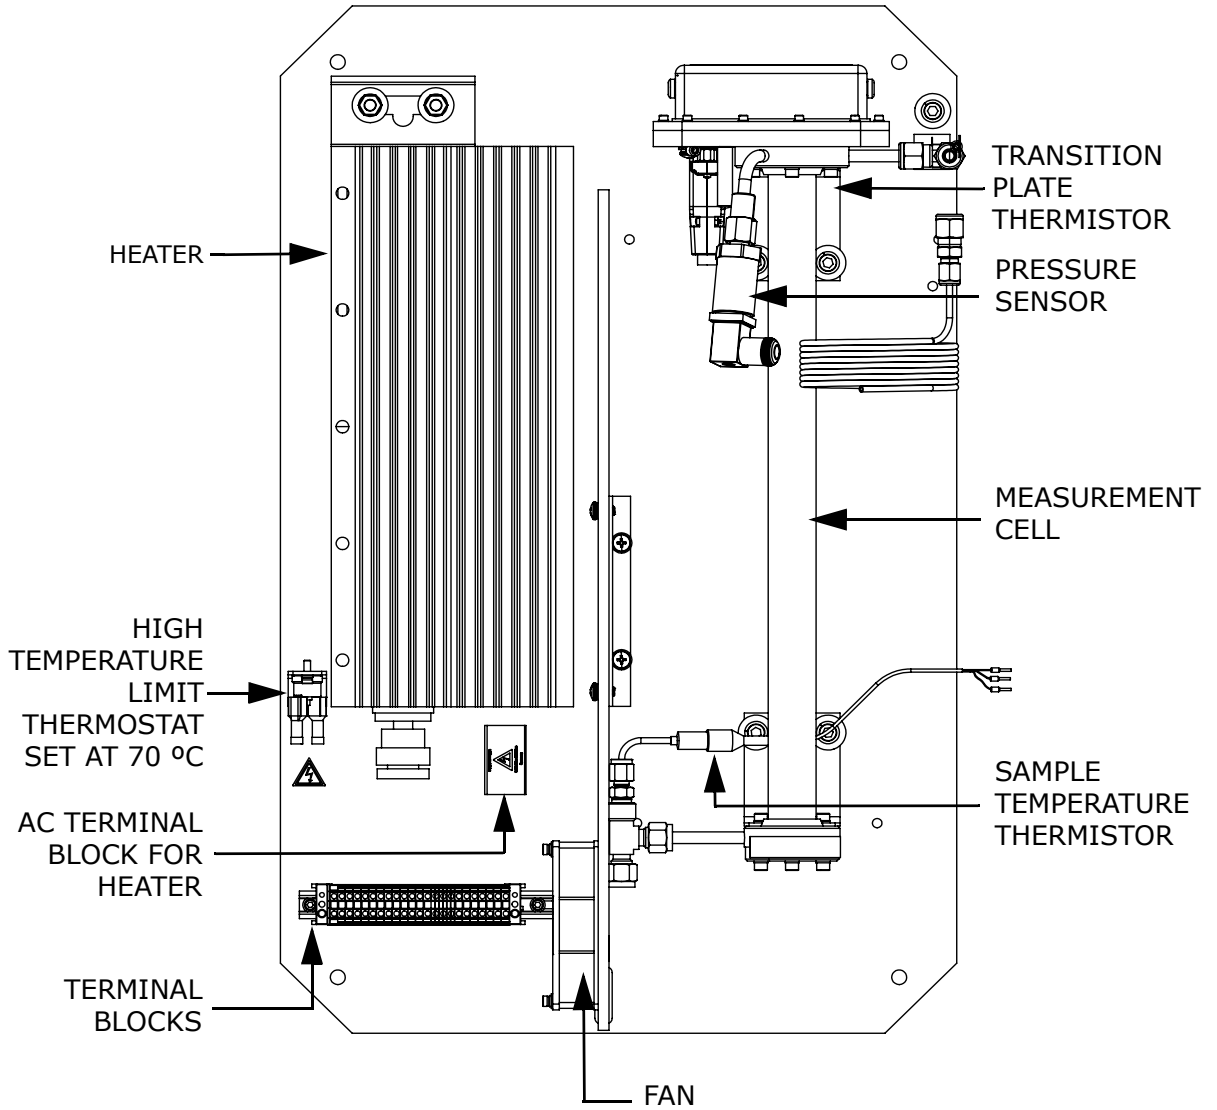


Figure 1-9 Components in 0.8 m sample cell enclosure

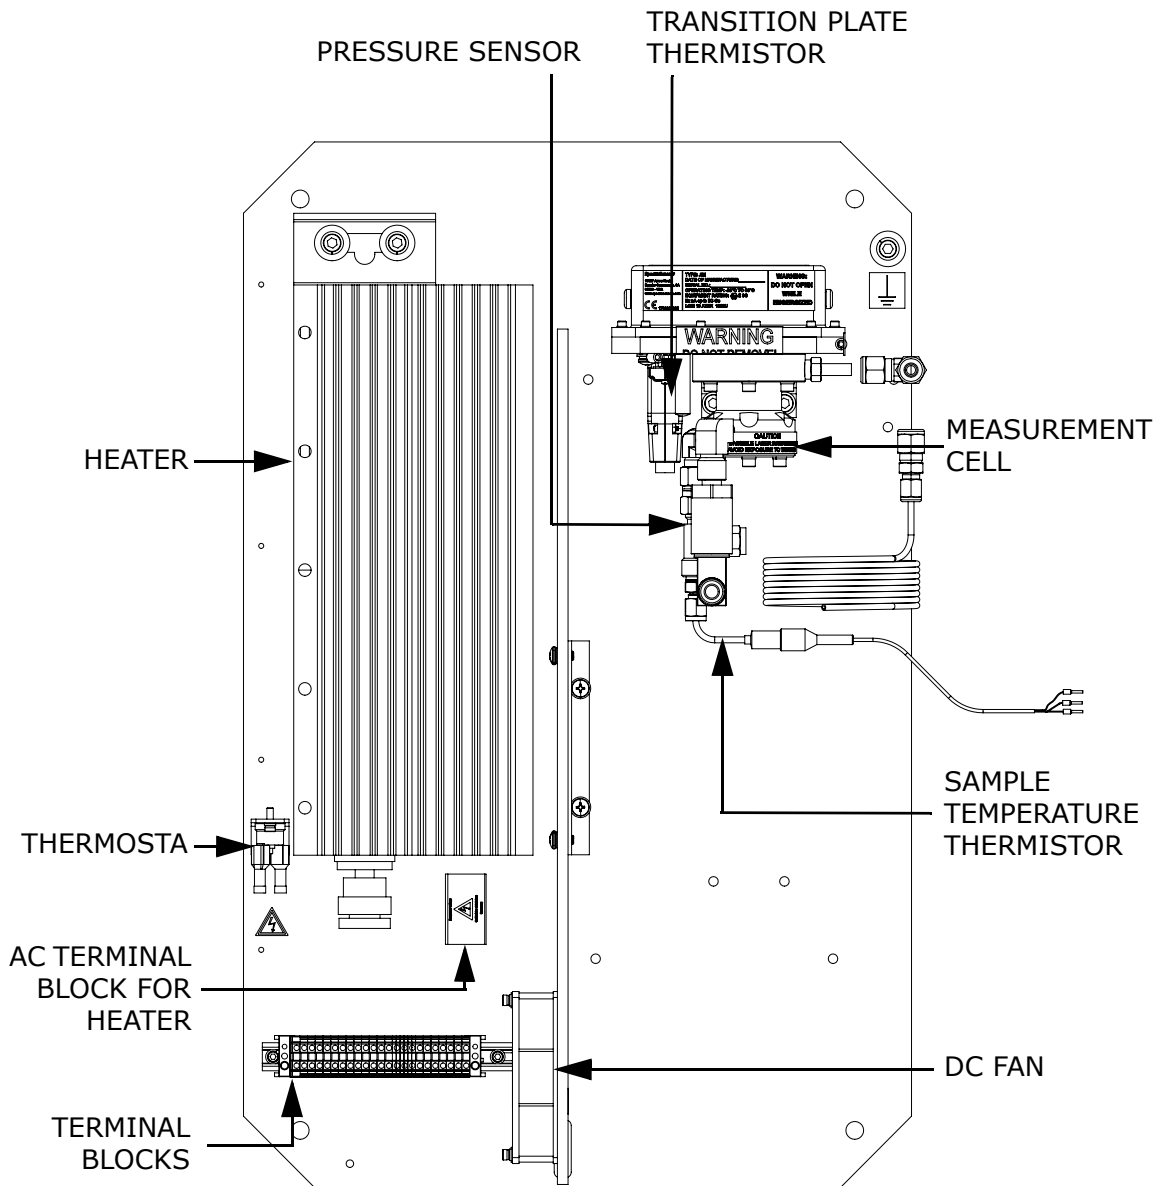


Figure 1-10 Components in 0.1 m sample cell enclosure

In the electronics enclosure, the analyzer power supply provides power to the analyzer control electronics and relays controlling valves. The analyzer control electronics drive the laser, collect the signal and analyze the spectra. Powered relays control valves while unpowered relays serve as alarm contacts. An AC line filter is used to condition the input power.

The auxiliary switch-mode power supply provides power to the heater temperature controller and the RS-232/RS-485 converter. The power supply is rated for 1.3A at 24VDC output at ambient temperatures $T_a \leq 60$ °C. The operational state is indicated by LEDs on the front face, where green means the output voltage is on and within specification, and red means the output voltage is on but below specification.

The thermostat prevents the temperature inside the enclosure from getting too hot. The thermostat is preset at the factory to open the power circuit if the temperature inside the analyzer enclosure exceeds 70 ± 4 °C. The power circuit will remain open until the manual reset button (located between the two wire terminals) on the thermostat is pressed or the temperature drops approximately 30% below the set-point.

A DIN rail near the bottom holds fuse terminal blocks, the main breaker and terminal blocks for all external connections. The temperature controller controls the heater in the sample cell enclosure via the solid-state relay.



See Figure 1-7 on page 1-11 for locating fuses. If you need to replace a fuse, use only the same type and rating of fuse as the original as listed in Table 1-1 below or Table 1-2 on page 1-16.

In the sample cell enclosure, the sample cell is the actual TDLAS spectrometer through which the gas sample flows. The sample cell is equipped with a pressure sensor and thermistor to monitor the thermodynamic conditions of the sample. The heater maintains the inside of the analyzer enclosure at a constant temperature with air circulated by the fan.

Table 1-1 Fuse specifications for 240 VAC systems

Drawing Reference	Description	Rating
F3	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 1.6A
F4 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 0.5A
F5 ¹ , F6 ¹ , F7 ¹ , F8 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 0.1A
F9 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 1.0A
F10 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 1.2A



1. Housed in fuse terminal blocks. Illuminated LED indicates blown fuse.

Table 1–2 Fuse specifications for 120 VAC systems




Drawing Reference	Description	Rating
F3	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 1.6A
F4 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 0.5A
F5 ¹ ,F6 ¹ ,F7 ¹ ,F8 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 0.1A
F9 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 1.0A
F10 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC 2.0A

1. Housed in fuse terminal blocks. Illuminated LED indicates blown fuse.

Special Safety Symbols Used on the Equipment

Special safety symbols and labeling are used on the equipment to alert the user to potential hazards and important information associated with the analyzer. Every symbol and label has significant meaning that should be heeded.

Refer to Figure 1–11 on page 1–18, Figure 1–12 on page 1–19, Figure 1–13 on page 20, Figure 1–14 on page 1–21 or Figure 1–15 on page 1–22 for label placement.



ENERGIZED FUSE WARNING - Do not remove or replace fuse when energized.



DO NOT REMOVE - Removal of the seal and/or disassembly of pieces traversed by label voids the warranty.



FUSE RATING - Maximum voltage and current specifications for the fuse closest to label.



HAZARDOUS VOLTAGE - Contact may cause electric shock or burn. Turn off and lock out system power before servicing.



GENERAL WARNING - Failure to follow all directions may result in damage or malfunction of the analyzer.



PROTECTIVE EARTH GROUND - Symbol indicates the connection point of the ground wire from the main power source.



FUNCTIONAL EARTH GROUND - Symbol indicates grounding points intended primarily for troubleshooting.



CLASS 1 LASER PRODUCT - Invisible laser radiation when open. Avoid direct exposure to the beam.



CLASS 3B LASER PRODUCT - Invisible laser radiation. Avoid direct exposure to beam. Class 3b laser product.



CLASS 3B LASER WARNING - Class 3B invisible laser radiation when open. Avoid direct exposure to the beam.

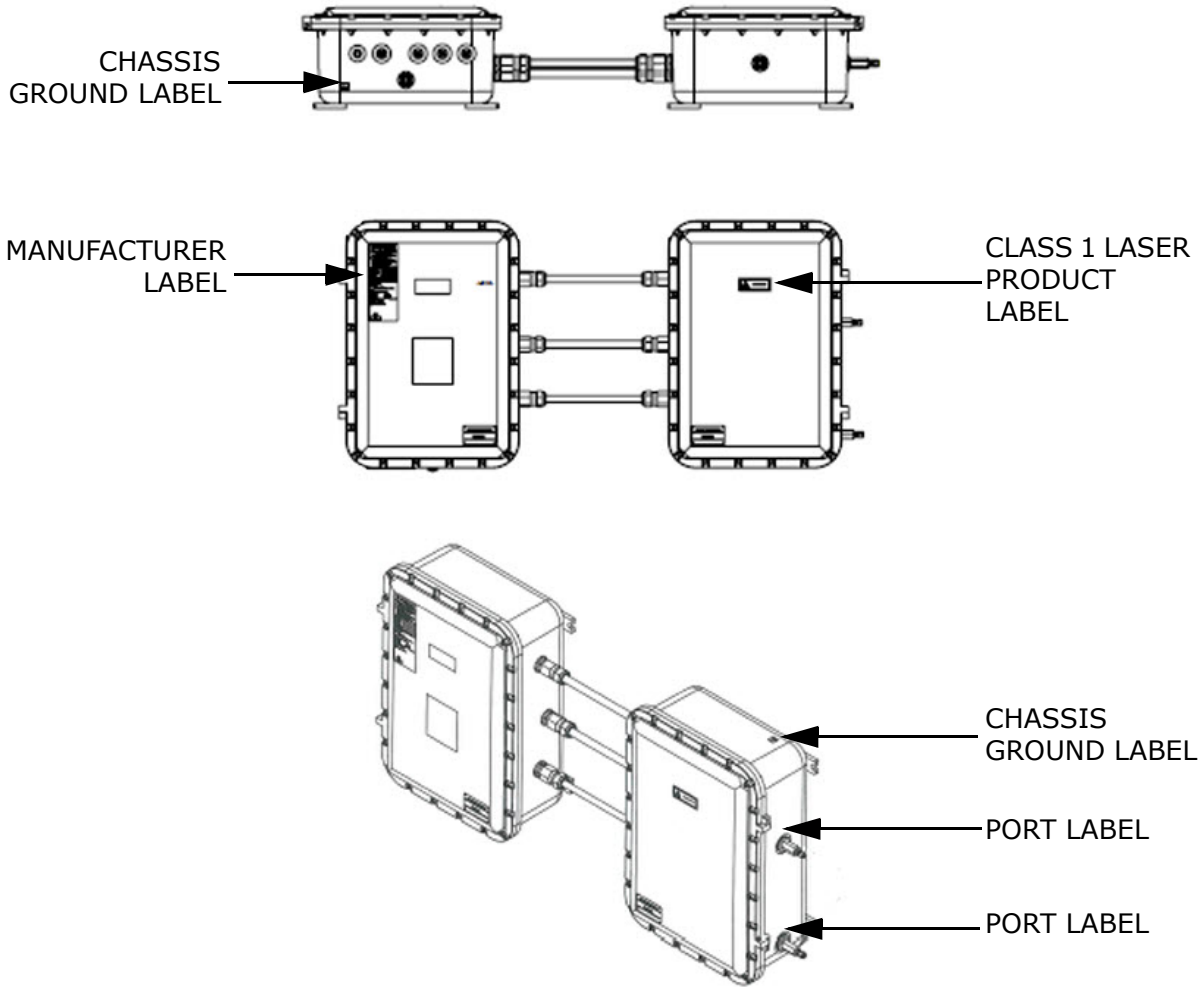


Figure 1-11 Label placement on exterior of enclosures

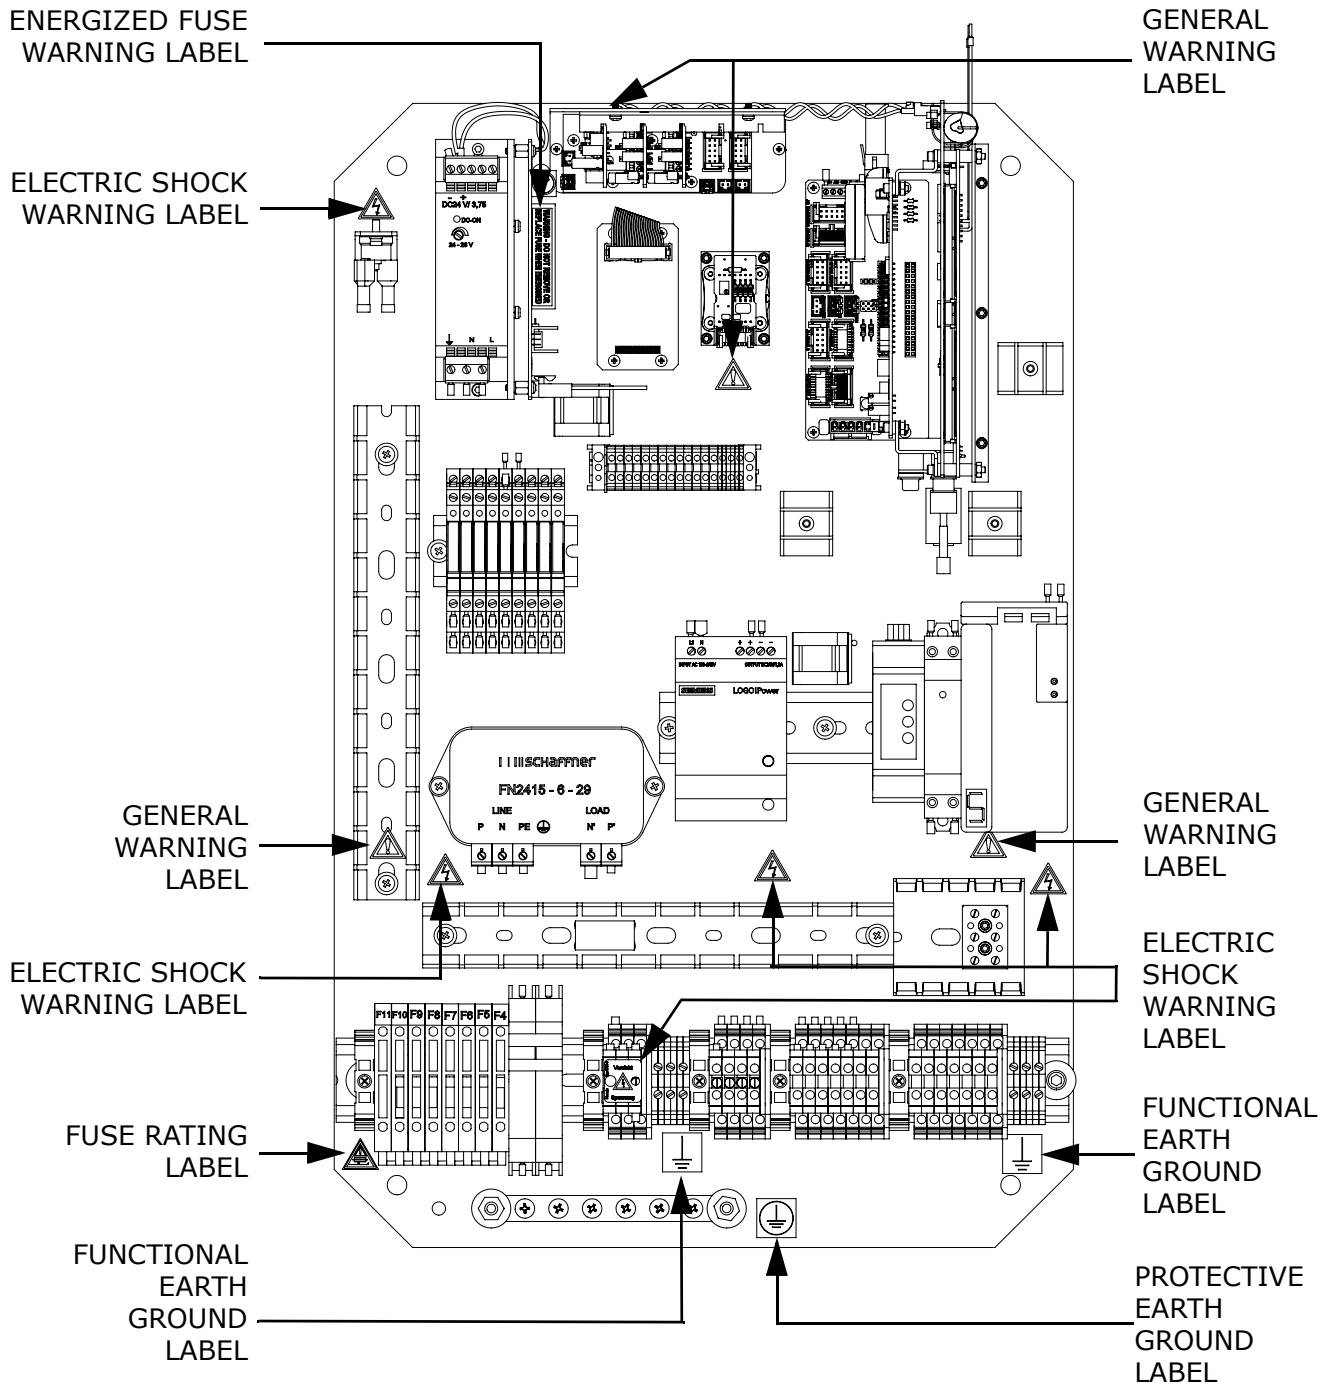


Figure 1-12 Label placement on electronics panel assembly

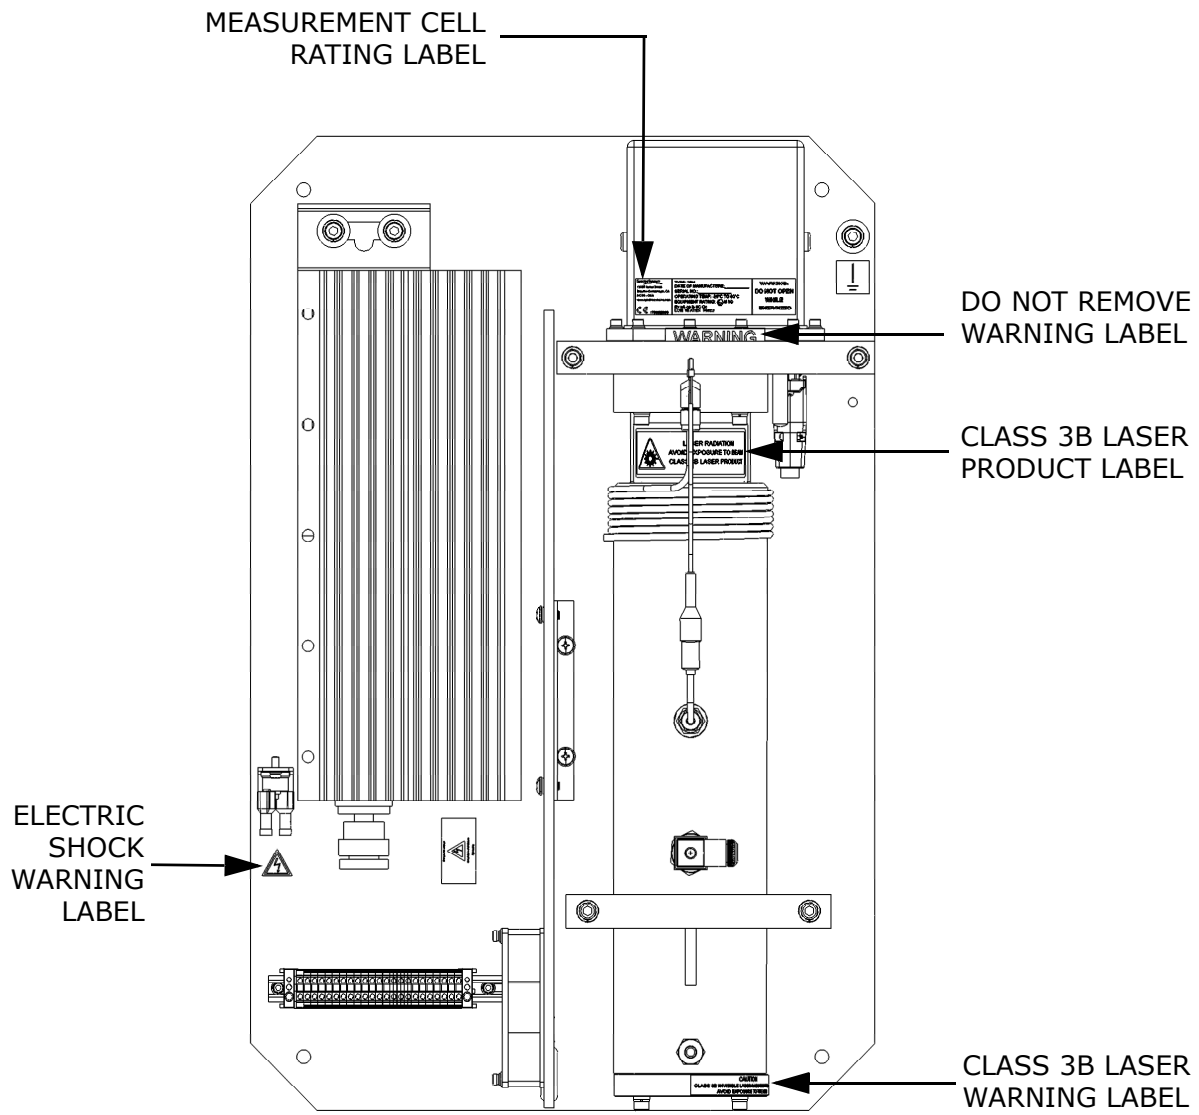


Figure 1-13 Label placement on 8/28 m sample cell panel

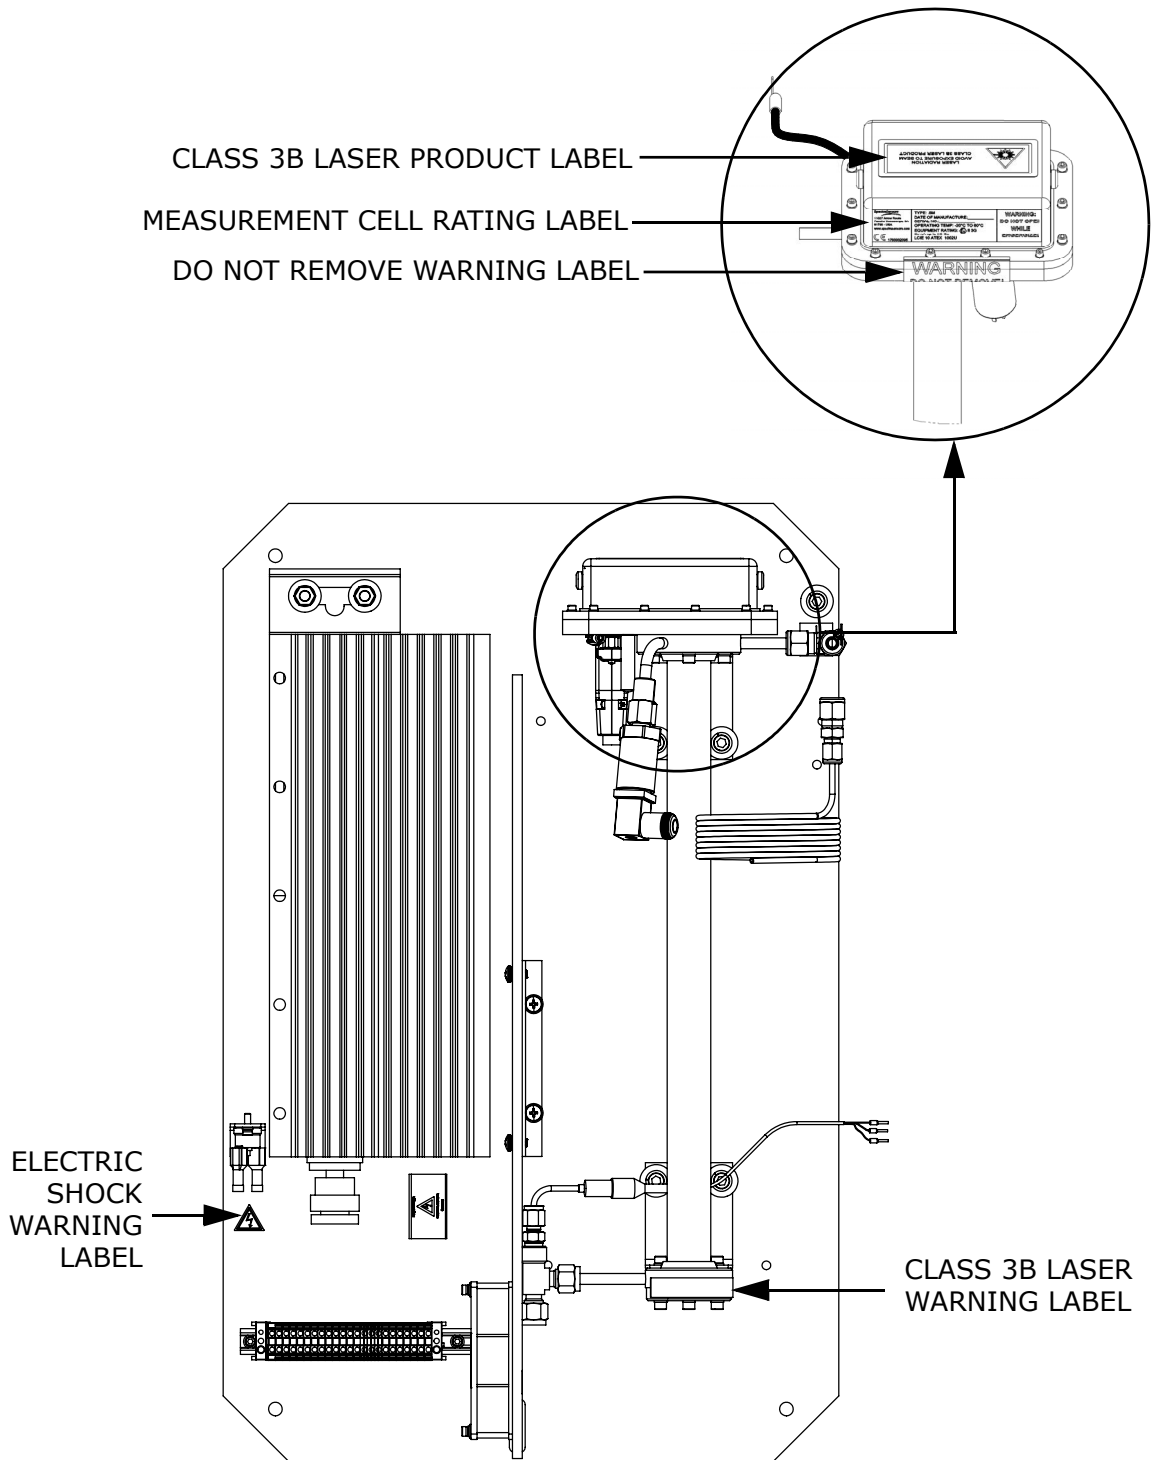


Figure 1-14 Label placement on 0.8 m sample cell panel

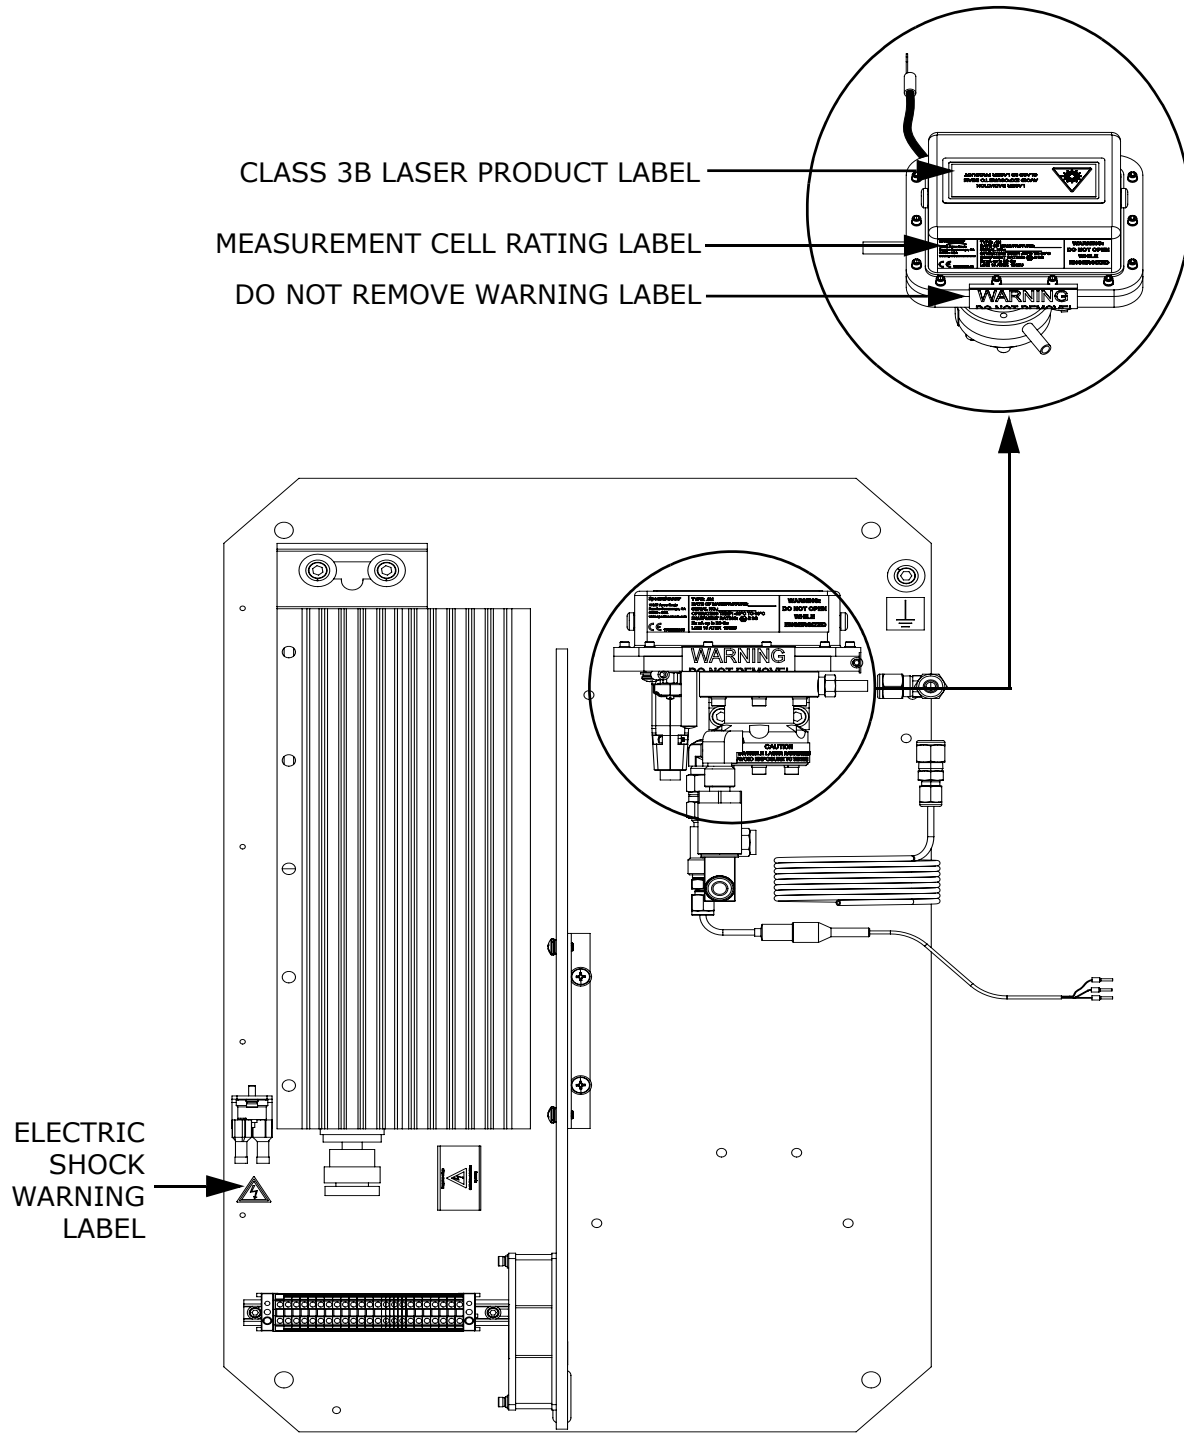


Figure 1-15 Label placement on sample cell panel assembly (0.1 m sample cell)

2 - SAFETY

Potential Risks Affecting Personnel

This section addresses the appropriate actions to undertake when faced with hazardous situations during or before service of the analyzer. It is not possible to list all potential hazards within this document. The user is responsible for identifying and mitigating any potential hazards present when servicing the analyzer.



Technicians are expected to follow all safety protocols established by the customer that are necessary for servicing the analyzer. This may include, but is not limited to, lockout/tag-out procedures, toxic gas monitoring protocols, PPE requirements, hot work permits and other precautions that address safety concerns related to performing service on process equipment located in hazardous areas.

Mitigating risks

Refer to the instructions for each situation listed below to mitigate associated risks.

Exposure to process gases

1. Shut off the process gas to the analyzer before any service that would require opening a part of the sample plumbing.
2. Purge the system with nitrogen.
3. Shut off the nitrogen purge before opening any part of the sample system.

Exposure to toxic gas (H₂S)

Follow the procedure below if there has been any suspected leak from the sample system and accumulated SCS enclosure.

1. Purge the SCS enclosure to remove any potentially toxic gas.
2. Test the H₂S levels of the SCS enclosure using the port from the safety purge kit to ensure the purge has cleared any toxic gas.
3. If no gas leak is detected, open the SCS enclosure door.



Follow all safety protocols governing toxic gases and potential leaks.

Electrocution hazard

1. Shut off power at the main disconnect external to the analyzer.



Complete this action before performing any service that requires working near the main input power or disconnecting any wiring or other electrical components.

2. Open enclosure door.

If service must be performed with power engaged (gain adjustment, etc.):

1. Note any live electrical components and avoid any contact with them.
2. Only use tools with a safety rating for protection against accidental contact with voltage up to 1000 V (IEC 900, ASTF-F1505-04, VDE 0682/201).

Explosion hazard

Any work in a hazardous area must be carefully controlled to avoid creating any possible ignition sources (e.g., heat, arcing, sparking, etc.). All tools must be appropriate for the area and hazards present. Electrical connections must not be made or broken with power on (to avoid arcing).

3 - INSTALLATION

This section describes the processes used to initially install and configure your SS2100i-2. Once the analyzer arrives, you should take a few minutes to examine the contents before installing the unit.

What Should be Included in the Shipping Box

The contents of the crate should include:

- The Endress+Hauser SS2100i-2 analyzer
- Document CDs; one that includes the Operating Instruction and another that includes the AMS100 software and instruction
- Tooling kit (P/N 1100002156)

If any of these contents are missing, contact your sales representative.

Lifting/Carrying the Analyzer

The SS2100i-2 is bolted on a Unistrut^a (or equivalent) metal frame in the factory. Due to the analyzer's size and weight (approximately 145 Kg [320 lbs], without sample conditioning system) Endress+Hauser recommends the use of a forklift, pallet jack, etc. to lift and/or move the analyzer.

Before removing from the crate, move the analyzer as close as possible to the final installation location. Always carry the load using the lifting eyes (refer to Figure 3-1 and the drawings included with the purchased SS2100i-2 analyzer).



Ensure all equipment used for lifting/moving the analyzer is rated for the maximum weight load.

Inspecting the Analyzer

Unpack and place the unit on a flat surface. Carefully inspect all enclosures for dents, dings, or general damage. Inspect the inlet and outlet connections for damage, such as bent tubing. Report any damage to the carrier.



Avoid jolting the instrument by dropping it or banging it against a hard surface, which may disturb the optical alignment.

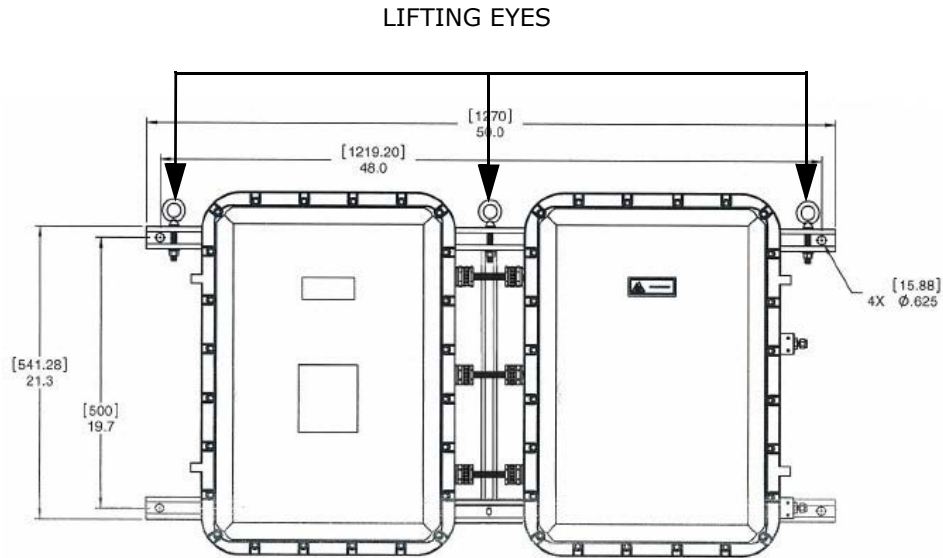


Figure 3-1 SS2100i-2 mounting and dimensions

Hardware and Tools for Installation

Depending on the particular model, the configuration of accessories and options ordered, you may need the following specific hardware and/or tools to complete the installation process.

Hardware

- Stainless steel tubing (Endress+Hauser recommends using 1/4 in. O.D. x 0.035 in. wall thickness, seamless stainless steel tubing)

Tools

- 8 mm hex key wrench
- 8 mm ball point hex L-key
- 10 mm ball point hex L-key
- 9/16 in. angle double open-end wrench - 15 degree and 75 degree
- 11/16 in. extra-long thin-head double open-end wrench
- 7/64 in. stainless steel ball point hex L-key
- 5/32 in. high torque ball point hex L-key
- RS-485 - USB converter (P/N 3100002220)

Mounting the Analyzer

Refer to the layout diagram in Appendix A or the system drawings delivered with the analyzer for mounting dimensions.



When mounting the analyzer, be sure not to position the instrument so that it is not difficult to operate adjacent devices. Allow 1 m (3 feet) of room in front of the analyzer and any switches.

To mount the analyzer:

1. Select a suitable location to mount the analyzer. Choose a shaded area or use an optional analyzer hood (or equivalent) to minimize sun exposure.



Endress+Hauser analyzers are designed for operation within the specified ambient temperature range. Intense sun exposure in some areas may cause the analyzer temperature to exceed the maximum.

2. Secure all designated attachment points.

Once all designated attachment points are securely fastened, the analyzer should be ready for the electrical connections.

Protective Chassis Ground Connections

Before connecting any electrical signal or power, the chassis grounds must be connected. Safety requirements for the protective and chassis grounds are as follows:

- The protective and chassis grounds must be of equal or greater size than any other current-carrying conductors, including the heater located in the sample conditioning system.
- The protective and chassis grounds must remain connected until all other wiring is removed.
- If the protective and chassis ground is insulated, it must use the green/yellow color.



Failure to properly ground the analyzer may create a high-voltage shock hazard.

Refer to Figure 1–6 for locations of the chassis ground connections.

1. Connect the chassis ground to the marked upper right corner of the right-side enclosure.

2. Connect the chassis ground to the marked bottom left corner of the left-side enclosure.
3. Connect the system ground to the ground bus bar as shown in Figure 1-7 during the electrical power connection.

Opening the Analyzer Enclosure Covers



Care must be taken to avoid damaging the enclosure cover and body mating surfaces which form a machined flame path (gap $\leq 0.05\text{mm}$, roughness $\leq 6\mu\text{m}$). If the surfaces are damaged to the extent they no longer meet the above specifications, please contact your Endress+Hauser service representative. Refer to Table B-1 on page B-23.

To open an analyzer enclosure cover

1. Using an 8 mm hex key wrench or driver, remove each cover screw completely.
2. Place cover screws in a safe place to protect against damage or loss.
3. Gently open cover by pulling on the edge opposite the hinges.

Cable Installation

To avoid potential damage, cable systems and accessories should be installed, so far as practicable, in positions that will prevent them from being exposed to mechanical damage, to corrosion or chemical influences, to the effects of heat and to UV radiation. Refer to the SS2100i-2 Safety Instruction (P/N XA02694C) for more information.

Terminations

Connections shall be made in a manner consistent with the type of terminal, type of protection and not introduce undue stress on the connections.

If multi-stranded and, in particular, fine-stranded conductors are employed, the ends shall be protected against separation of the strands, e.g., by means of cable lugs, core-end sleeves or by the type of terminal, but not by soldering alone.



The creepage distances and clearances shall not be reduced by the method in which the conductors are connected to the terminals.

Cable Glands



Certified compound barrier seal type glands and cables shall be used where appropriate in compliance with local regulations.

The cable gland shall be selected to match the cable diameter. The use of sealing tape, heat-shrink tube or other materials are not permitted to make the cable fit to the cable gland.

If an Ex "d" gland clamping by the sealing ring (compression) is used with braided or armored cable, it shall be the type where the braid or armor is terminated in the gland and compression takes place on the inner cable sheath.



For flameproof enclosures, adapters shall not be used together with blanking elements.

Flameproof cable glands, adapters or blanking elements, having parallel threads may be fitted with a sealing washer between the entry device and the flameproof enclosure provided that the applicable thread engagement is still achieved after the washer has been fitted. Thread engagement shall be at least five (5) full threads. Suitable grease may be used as long as it is non-setting, non-metallic and non-combustible and any earthing between the device and the flameproof enclosure is maintained. Endress+Hauser recommends using STL8 screw thread lubricant or equivalent on all screw thread and its taped opening. Refer to "**Application of Gland Lubricant**" on page 3-11.



Do not use this lubricant on exposed current-carrying parts.

Unused cable entries shall be sealed with a flameproof blanking element, which shall be fitted directly to the hole (no threaded adapter shall be used), and shall comply with thread engagement requirements detailed above and shall be secured against loosening.

Connecting the Solenoid Valves

Differential systems require solenoid valves to switch between process flow and flow that has been scrubbed of the analyte. The solenoids switch the flow either directly, as shown in Figure 3-2, or via instrument air driving pneumatic valves, as shown in Figure 3-3 through Figure 3-5. Refer to "**Differential TDLAS**" on page 1-7.

For systems performing differential measurements that do not have a factory installed sample system, the cables connecting the solenoid valve(s) to the

electronics must be installed. All work should be performed by personnel qualified in electrical installation.



Pay special attention to systems measuring especially reactive or adherent species. Because of the reactive or adherent nature of such species, accurate measurement of their concentration may be compromised somewhat by adsorption, desorption or reaction with wetted surfaces. Special coatings are available to minimize these effects.



An appropriate sample conditioning system that has been specifically designed to deliver a sample stream that is representative of the process stream at the time of sampling should be used with the system to assure that the analyzer is receiving sample gas that can be correctly measured.

A schematic of a typical basic differential setup for installations where no instrument air is available to drive pneumatic valves is shown in Figure 3-2. A more preferable setup is shown in Figure 3-3 where only one solenoid is required in favor of more reliable pneumatic valves. Systems set up for auto-validation with one gas require two solenoids, as shown in Figure 3-4, whereas auto-validation with two gases requires four solenoids, as shown in Figure 3-5.



Certified compound barrier seal glands and braided armored cables should be used where appropriate in compliance with local regulations.



Hazardous voltage and risk of electric shock. Turn off and lock out system power before opening the electronics enclosure and making any connections.



Be sure to use solenoid valves rated for the output voltage of the relays on your system. Failure to do so may result in fire.

To connect the solenoid valves

1. Open the analyzer enclosure cover according to the procedure under **"To open an analyzer enclosure cover"** on page 3-4 to gain access to the field interface terminal block.
2. Install an appropriate compound barrier seal type gland into the M25 access port on the bottom left of the enclosure. Refer to **"Application of Gland Lubricant"** on page 3-11.
3. Pull the solenoid valve cables into the electronics enclosure.

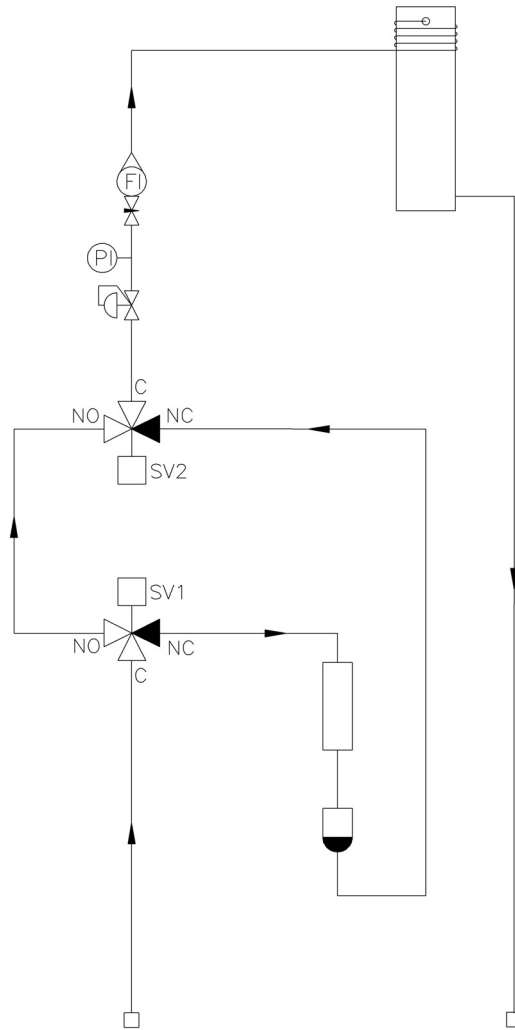


Figure 3-2 Basic differential system with two solenoid valves

4. Strip back the jacket and insulation of the solenoid valve cables just enough to connect to the appropriate terminals on the field interface terminal block for your particular sample conditioning scheme, as indicated in Table 3-1.

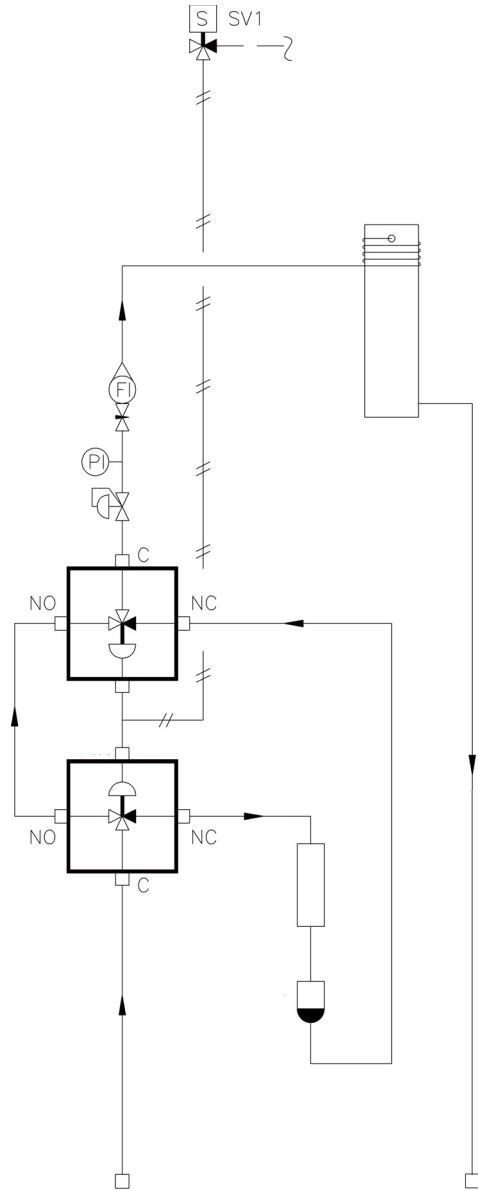


Figure 3-3 Preferred basic differential system with one solenoid valve driving two pneumatic valves

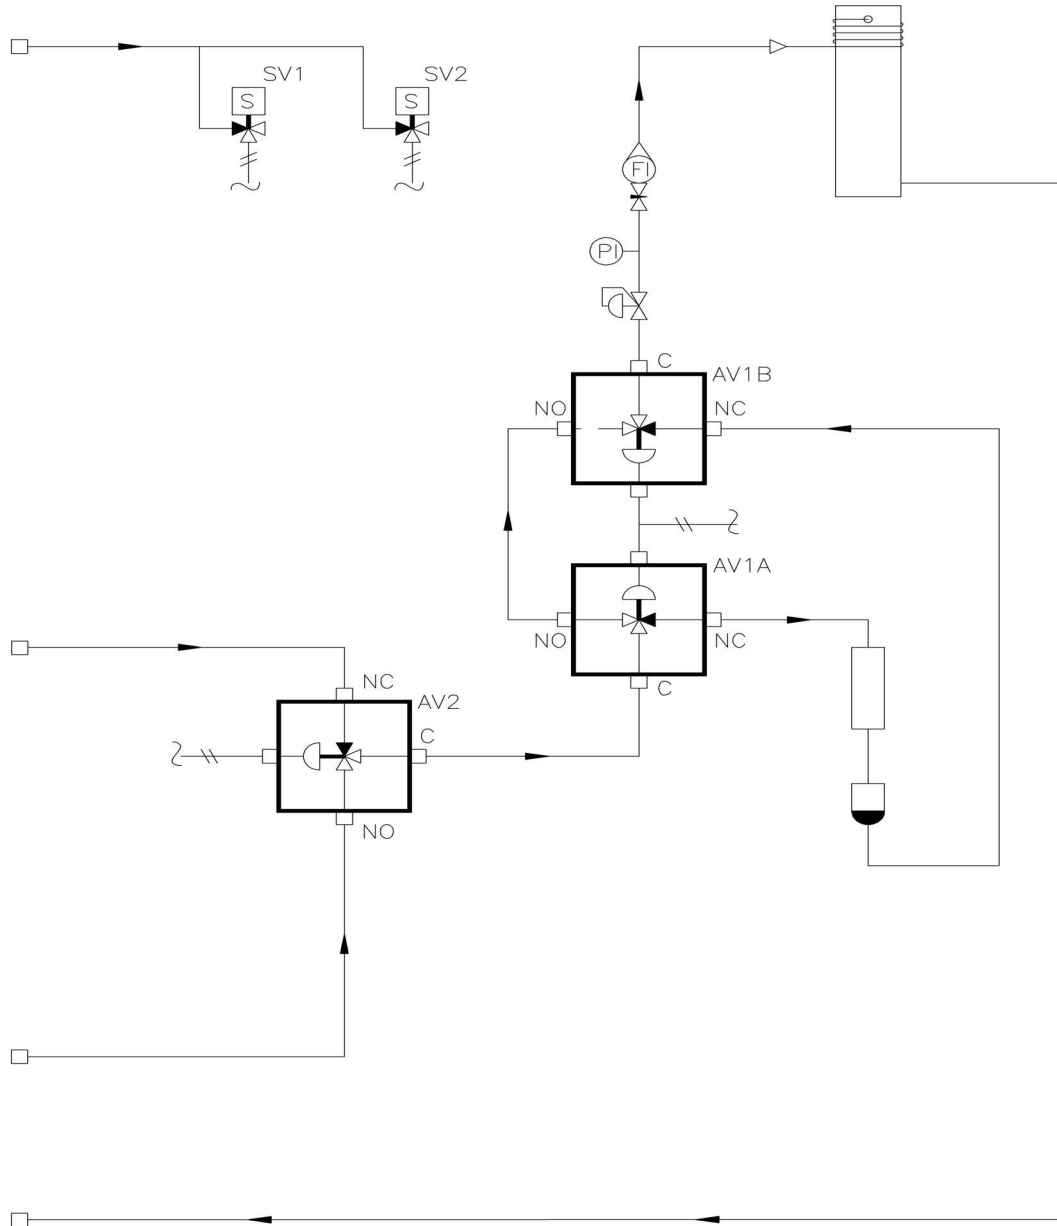


Figure 3-4 Differential system with single auto-validation requiring two solenoid valves driving three pneumatic valves

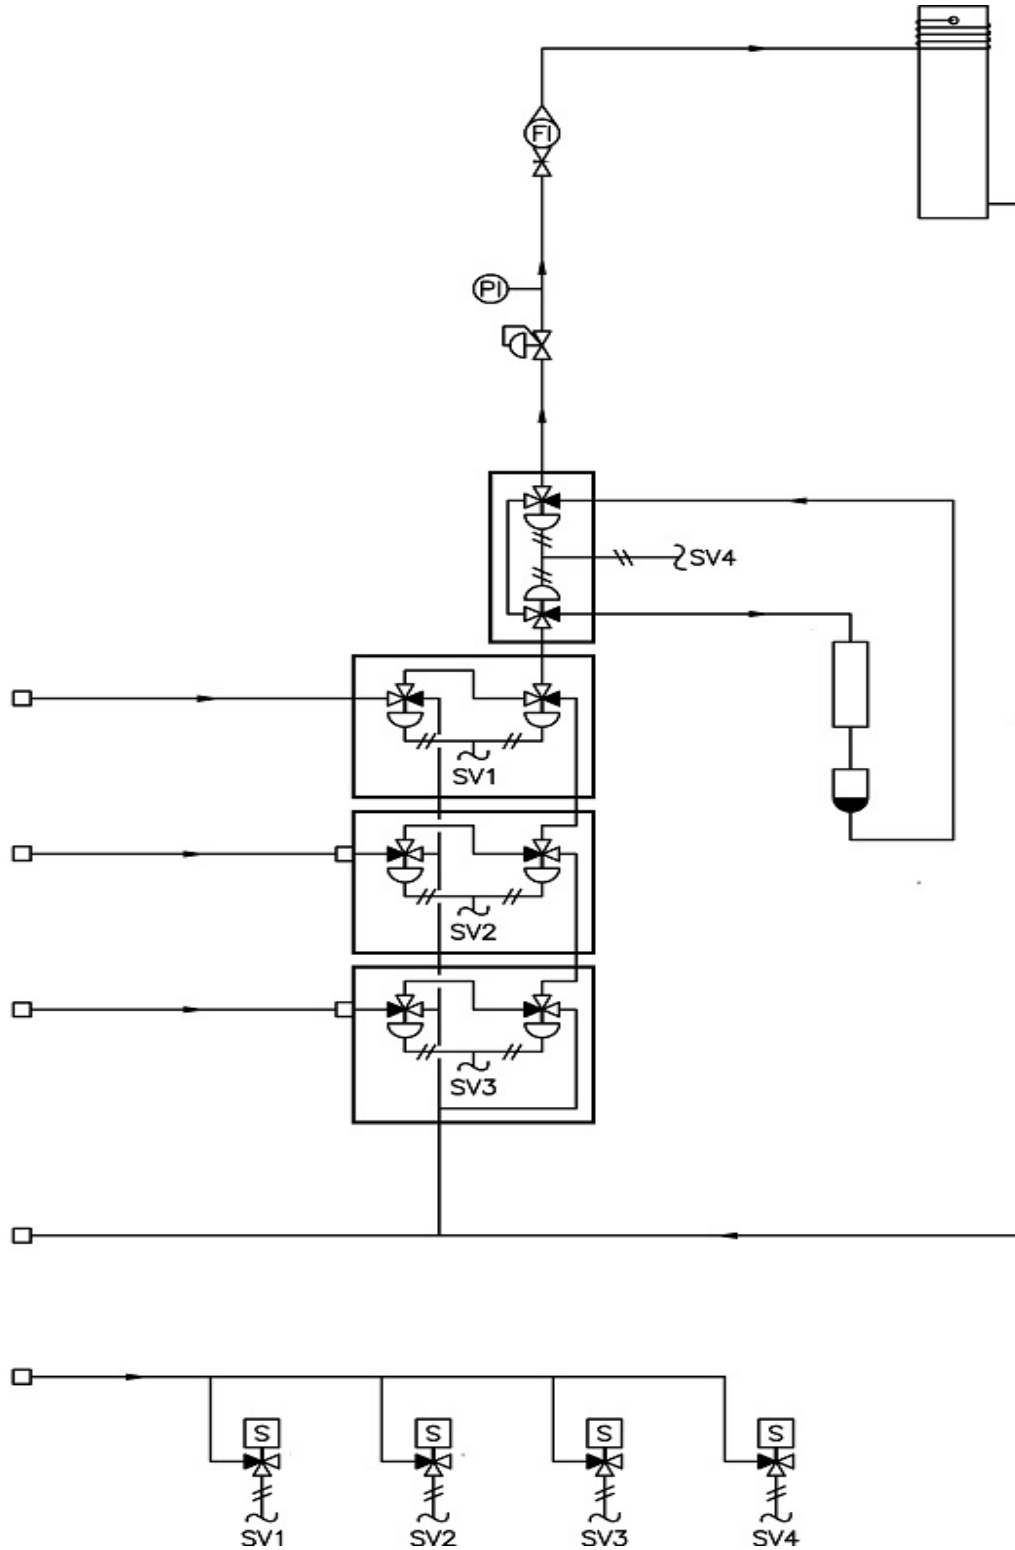


Figure 3-5 Differential system with dual auto-validation requiring four solenoid valves driving eight pneumatic valves

NOTE: For valve configurations refer to Figure 3-2 through Figure 3-5.

Table 3-1 Terminal block (X2) solenoid valve connections

Fig.	SOV	Description	Terminal	Relay Rating
				I_{th}
3-2	S1	Scrubber Solenoid	1	6A
			2	
	S2	Main/Val Solenoid	3	
			4	
3-3	S1	Scrubber Solenoid	1	
			2	
3-4	S1	Scrubber Solenoid	1	
			2	
	S2	Val 1 Solenoid	5	
			6	
3-5	S1	Scrubber Solenoid	1	
			2	
	S2	Main/Val Solenoid	3	
			4	
	S3	Val 1 Solenoid	5	
			6	
	S4	Val 2 Solenoid	7	
			8	

5. Verify that each connection is secure.
6. Close the analyzer enclosure cover.

Application of Gland Lubricant

To ensure proper installation, Endress+Hauser recommends using STL8 screw thread lubricant or equivalent on all conduit screw thread and its taped opening.

STL8 Screw Thread Lubricant is a lithium based, anti-galling substance with excellent adhesion that maintains rain-tightness and grounding continuity

between conduit fittings. This lubricant has proven very effective between parts made of dissimilar metals, and is stable in temperatures from -20 °F to +300 °F.



Do not use this lubricant on exposed current-carrying parts.

1. Holding the fitting piece at one end, generously apply the lubricant on the male threaded surface (at least five threads wide) as shown below.



Figure 3-6 *Applying conduit lubricant*

2. Screw the female pipe thread onto the male fitting until the lubricated threads are engaged.

Eyes: *May cause minor irritation.*



Skin: *May cause minor irritation.*

Ingestion: *Relatively non-toxic. Ingestion may result in a laxative effect. Ingestion of substantial quantities may cause lithium toxicity.*

Connecting the Signals and Alarms

The 4 to 20 mA AI, 4 to 20 mA AO, serial and Ethernet outputs are connected to terminal block (X4), as shown in Figure 3-7. In addition, seven digital inputs/outputs connected to SPDT relays through terminal block (X3) are also provided.

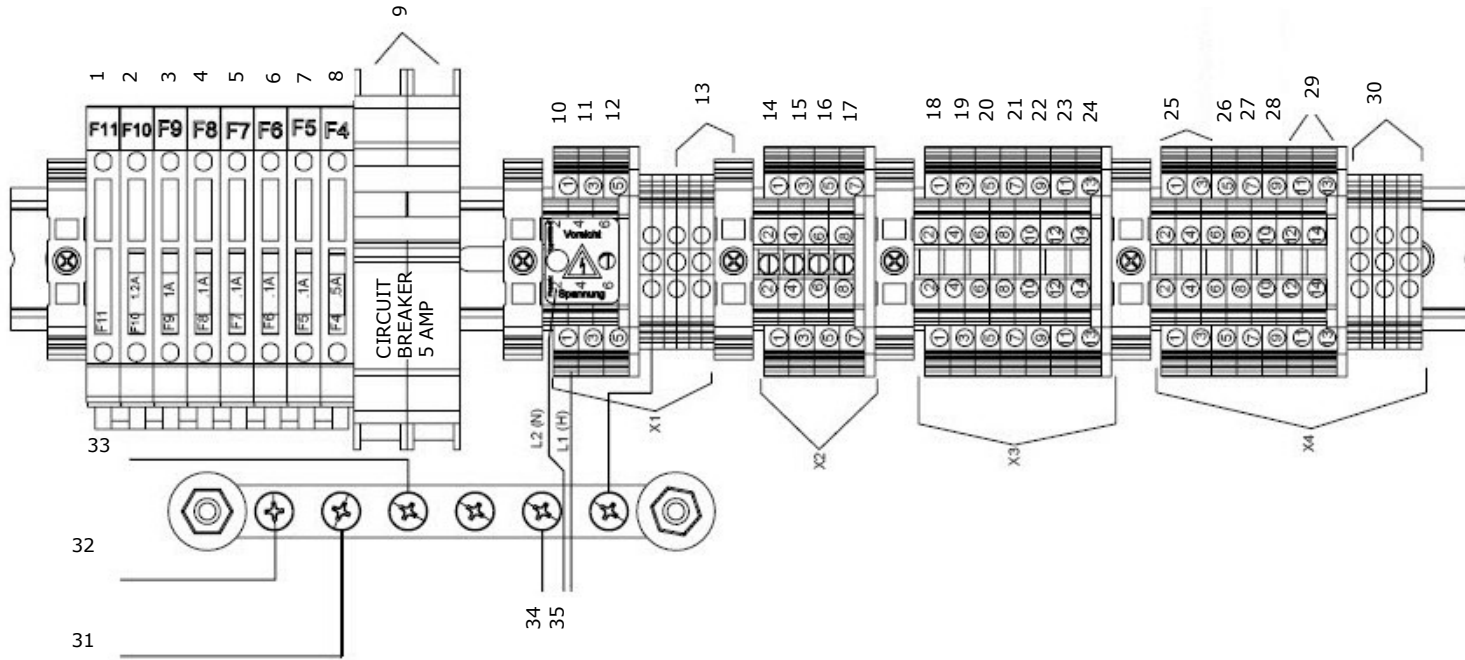


Figure 3-7 Field interface terminal block for connection of input power and input/output signals

- | | | | |
|-------------------------------------|---|---|--|
| 1 Spare | 11 Heater Neutral Terminal 4 | 20 VAL Fail to Customer Terminal 5,6 | 28 4-20 mA Input Terminal 9,10 |
| 2 To Temp Limit Sw Heater | 12 AC, Filter Terminal 6 | 21 VAL 1 Active to Customer Terminal 7,8 | 29 Ethernet Output Terminal 11,12,13,14 |
| 3 To ABB Power Supply (G3) | 13 Ground Terminals | 22 VAL 2 Active to Customer Terminal 9,10 | 30 4-20 mA and Serial Cable Ground Terminals |
| 4 To K4-14 | 14 Scrubber Terminal 1,2 (SV1,SV2) | 23 Flow Switch from Customer Terminal 11,12 | 31 From Enclosure Ground Stud |
| 5 To K3-14 | 15 N.O. Connection (N/C) | 24 VAL REQ from Customer Terminal 13,14 | 32 From Enclosure Door Ground Stud |
| 6 To K2-14 | 16 VAL 1 Terminal 5,6 | 25 RS-485 Output Terminals 1,2,3,4 | 33 From Heater Ground Stud |
| 7 To K1-14 | 17 VAL 2 Terminal 7,8 | 26 CH A 4-20 mA Output Terminal 5,6 | 34 PE |
| 8 To ABB Power Supply (G3) | 18 HI Alarm CH2 TO Customer Terminal 1,2 | 27 CH B 4-20 mA Output Terminal 7,8 | 35 Incoming Power |
| 9 To AC Filter | 19 General Alarm to Customer Terminal 3,4 | | |
| 10 To Circuit Breaker Terminals 1,2 | | | |



*The 4 to 20 mA current loop output is factory set to source current. To change the 4 to 20 mA current loop output from source to sink, see **"To change the 4 to 20 mA board from source to sink"** on page 3-20.*

The relays for the alarms are configured to be fail-safe (or normally energized) so the dry contacts will open in the event of power loss. Thus, the alarms are wired to be normally closed (NC) when the analyzer is running.

Consult the wiring diagrams in Appendix D. All work should be performed by personnel qualified in electrical installation.



Certified compound barrier seal glands and cables shall be used where appropriate in compliance with local regulations.









Hazardous voltage and risk of electric shock. Turn off and lock out system power before opening the electronics enclosure and making any connections.

To connect the signal and alarm cables

- 1.** Open the enclosure cover according to the procedure under **"To open an analyzer enclosure cover"** on page 3-4 to gain access to the field interface terminal block.
- 2.** Install appropriate compound barrier or seal type glands into the three M25 access ports on the bottom right of the electronics enclosure. Refer to **"Application of Gland Lubricant"** on page 3-11.
- 3.** Pull the cables for the alarm outputs and validation request input through the first (from left) gland, the cables for the 4 to 20 mA AI and 4 to 20 mA AO through the second gland and the cable for serial or Ethernet communication through the third gland and into the enclosure.
- 4.** Strip back the jacket and insulation of the 4 to 20 mA AI, 4 to 20 mA AO and serial or Ethernet cables just enough to connect to the terminals of block (X4).
- 5.** Connect the 4 to 20 mA AI, 4 to 20 mA AO and serial or Ethernet wires to the appropriate terminals, as indicated in Table 3-2.

NOTE: The description "N/C" means no connection.

Table 3-2 Terminal block (X4) input/output signal connections

Terminal	Description	D Pin #	Wire Color Cat5(e)		
1	Serial Rx or TD-	1	Blue 		
2	Serial Tx or TD+	2	Brown 		
3	N/C				
4	N/C				
5	4 to 20 mA AO Ch. A (+)				
6	4 to 20 mA AO Ch. A (-)				
7	4 to 20 mA AO Ch. B (+)				
8	4 to 20 mA AO Ch. B (-)				
9	4 to 20 mA AI (+)			RJ45 Pin #	Wire Color (T568B) Cat5(e)
10	4 to 20 mA AI (-)				
11	Ethernet Tx+ (BI_DA+)	1	White/Orange 		
12	Ethernet Tx- (BI_DA-)	2	Orange 		
13	Ethernet Rx+ (BI_DB+)	3	White/Green 		
14	Ethernet Rx- (BI_DB-)	6	Green 		
G	Serial Shield Ground				
G	4 to 20 mA Ch. A Shield GND				
G	4 to 20 mA Ch. B Shield GND				

6. Strip back the jacket and insulation of the alarm output and validation request input cables just enough to connect to the terminals of block (X3).
7. Connect the alarm output and validation request input wires to the appropriate terminals, as indicated in Table 3-3.
8. Verify that each connection is secure.
9. Close the analyzer enclosure cover.
10. To complete the connections, connect the other end of the current loop wires to a current loop receiver, the serial or Ethernet to a serial or Ethernet port on a computer, the alarm cables to appropriate alarm monitors and the validation request input to a switch.

Table 3-3 Terminal block (X3) input/output signal connections

Terminal	Description
1	High Concentration Alarm
2	
3	General Fault Alarm
4	
5	Validation Fail Alarm
6	
7	Validation 1 Active
8	
9	Validation 2 Active
10	
11	Future Use
12	
13	Validation Request Input
14	

Configuring the RS-232/RS-485 Converter

The Optically Isolated RS-232 to RS-485 Converter is configured for two-wire RS-485. DIP switches on the side of the converter, shown in Figure 3-8, can be used to set time-out and termination.

Refer to Table 3-4. With the default setting of 9600 baud, the converter will generally work for baud rates of 9600 and higher.

Connecting Electrical Power to the Analyzer

The analyzer will be configured for 120 or 240 VAC @ 50/60 Hz single phase input. Check the manufacturing data label or the terminal block labels to determine the power input requirements. All work should be performed by personnel qualified in electrical installation.

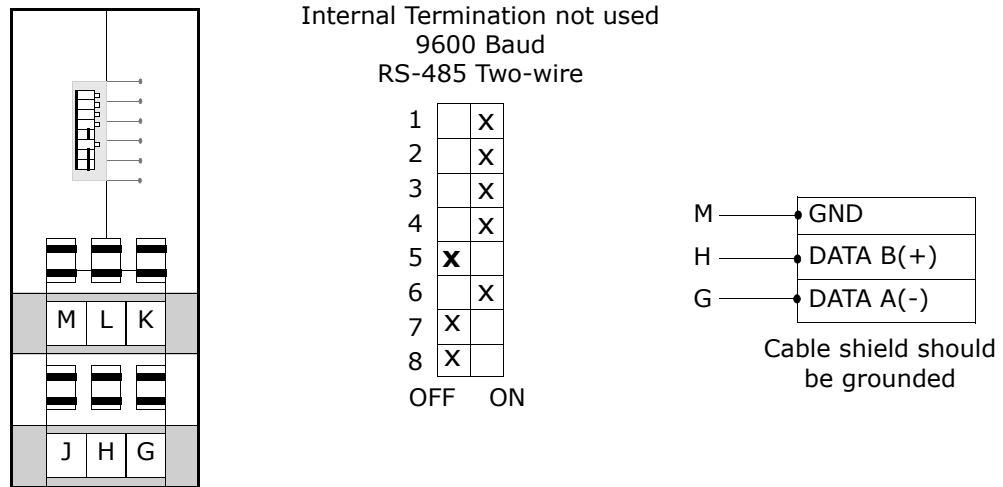


Figure 3-8 Optically isolated RS-232-to-RS-485 converter DIP switches

Table 3-4 Output signal connections (two-wire RS-485 configuration)

	SW1	SW2	SW3	SW4	SW5	SW6	SW7	SW8	Time-out ¹ (ms)	R11 (KΩ)
RS-485 2-Wire Half Duplex	ON	ON	ON	ON						
120Ω Built-in Termination					ON					
External or no Termination					OFF					
1200 Baud						OFF	OFF	OFF	8.330 ²	820
2400 Baud						OFF	OFF	ON	4.160	
4800 Baud						OFF	ON	OFF	2.080	
9600 Baud						ON	OFF	OFF	1.040	
19.2K Baud						ON	ON	ON	0.580	
38.4K Baud						OFF	OFF	OFF	0.260 ²	27
57.6K Baud						OFF	OFF	OFF	0.176 ²	16
115.2K Baud						OFF	OFF	OFF	0.087 ²	8.2

1. Time-out selections are equal to one character time at the indicated baud rate.
2. To achieve this time-out, an appropriate through-hole resistor must be placed in the R11 location on the converter PCB.



Hazardous voltage and risk of electric shock. Turn off and lock out system power before opening the electronics enclosure and making any connections.



Certified compound barrier seal type glands and cables shall be used where appropriate in compliance with local regulations.



See Figure 1-7 on page 1-11 for locating fuses. If you need to replace a fuse, use only the same type and rating of fuse as the original as shown in Table 3-5 and Table 3-6. For re-order part numbers, refer to Table C-2 on page C-5.

Table 3-5 Fuse specifications for 240 VAC systems

DWG Ref.	Description	Rating
F3	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/1.6A
F4 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/0.5A
F5 ¹ ,F6 ¹ ,F7 ¹ ,F8 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/0.1A
F9 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/1.0A
F10 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/1.2A



1. Housed in fuse terminal blocks. Illuminated LED indicates blown fuse.

NOTE: Refer to the drawing in Figure 1-7.

Table 3-6 Fuse specifications for 120 VAC systems

DWG Ref.	Description	Rating
F3	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/1.6A
F4 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/0.5A
F5 ¹ ,F6 ¹ ,F7 ¹ ,F8 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/0.1A
F9 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/1.0A
F10 ¹	Miniature Fuse, 5 x 20 mm, Time Delay	250 VAC/2.0A



1. Housed in fuse terminal blocks. Illuminated LED indicates blown fuse.

NOTE: Refer to the drawing in Figure 1-7.

To connect electrical power to the analyzer

1. Open the analyzer enclosure cover according to the procedure under **"To open an analyzer enclosure cover"** on page 3-4 to gain access to the field interface terminal block.
2. Install an appropriate compound barrier seal type gland into the M20 access port on the bottom left of the electronics enclosure. Refer to **"Application of Gland Lubricant"** on page 3-11.
3. Run cable from the power distribution panel to the gland.



An approved switch or circuit breaker rated for 15 amps should be used and clearly marked as the disconnecting device for the analyzer.



Because the breaker in the power distribution panel or switch will be the primary means of disconnecting the power from the analyzer, the power distribution panel or switch should be located in close proximity to the equipment and within easy reach of the operator.

4. Pull ground, neutral and hot wires (#14 AWG minimum) into the analyzer enclosure.
5. Strip back the jacket and/or insulation of the wires just enough to connect to the power terminal blocks (X1).
6. Attach the neutral and hot wires to the power terminal blocks by connecting the neutral wire to terminal X1-2, the hot wire to terminal X1-1, as shown in Figure 3-7.
7. Connect the ground wire to the ground bus bar marked \oplus .



Failure to properly ground the analyzer may create a high-voltage shock hazard.

8. Verify that each connection is secure.
9. Close the analyzer enclosure cover.

Connecting the Gas Lines

Once you have verified that the analyzer is properly wired, you are ready to connect the sample supply and sample return lines. All work should be performed by technicians qualified in pneumatic tubing.

Endress+Hauser recommends using 1/4 in. O.D. x 0.035 in. wall thickness, seamless stainless steel tubing. If the analyzer comes with a factory installed

sample system, consult the system drawings for tubing sizes and attachment points.



For systems with integral sample conditioning systems, refer to the sample system manual.

To connect the sample supply and return lines

1. Connect the supply and return tubes to the analyzer using the stainless steel compression-type fittings provided.
2. Tighten all new fittings 1-1/4 turns with a wrench from finger tight. For connections with previously swaged ferrules, thread the nut to the previously pulled up position, then tighten slightly with a wrench. Secure tubing to appropriate structural supports as required.
3. Check all connections for gas leaks. Endress+Hauser recommends using a liquid leak detector.



Do not exceed 10 PSIG (0.7 barg) in sample cell. Damage to cell may result.

Changing the 4 to 20 mA Current Loop Mode



Changing the current loop mode may negate specific hazardous area certifications.

By default, the 4 to 20 mA current loop output is factory set to source current. In some instances it may be necessary to change the 4 to 20 mA current loop output in the field from source to sink. This work should be performed by personnel qualified in electronics assembly.



Hazardous voltage and risk of electric shock. Turn off and lock out system power before opening the electronics enclosure and servicing.

To change the 4 to 20 mA board from source to sink

1. Disconnect power to the analyzer.

2. Open the analyzer enclosure cover according to the procedure under **"To open an analyzer enclosure cover"** on page 3-4 to gain access to the electronics panel.
3. Locate the 4 to 20 mA current loop board in the upper middle of the electronics panel, as shown in Figure 1-7.
4. Unscrew the screws holding the retaining bracket and remove the retaining bracket.
5. Gently pull the 4 to 20 mA current loop board up off the backplane into which it is plugged.
6. Move the jumper (JMP1) connecting the center pin to pin A, shown in Figure 3-9, to connect the center pin with pin P.

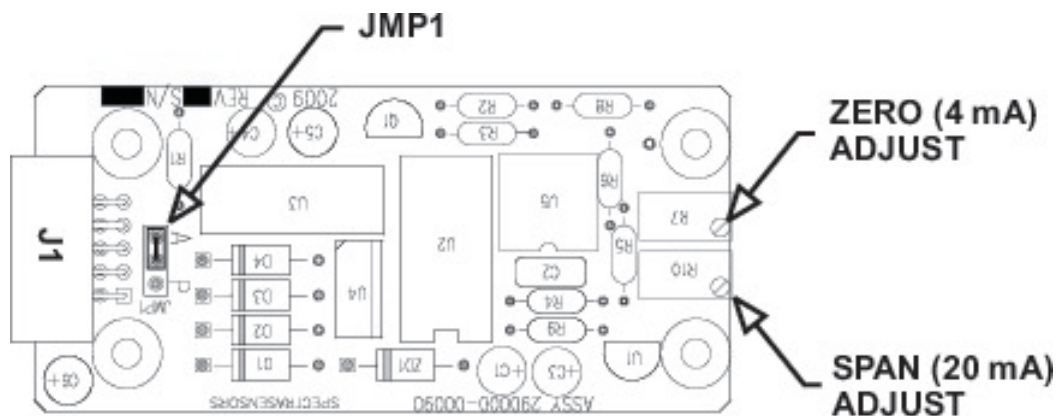


Figure 3-9 4 to 20 mA board

7. Re-install the 4 to 20 mA current loop board and retaining bracket.
8. Reconnect power to the analyzer. Confirm the 4 mA (min.) and 20 mA (max.) points (refer to the appropriate chapter in the Description of Device Parameters for **"Scaling and Calibrating the Current Loop Signal"**).
9. Close the analyzer enclosure cover.

THIS PAGE INTENTIONALLY LEFT BLANK

Appendix A: Specifications




Table A-1 SS2100i-2 analyzer specifications

Performance	
Concentration	See analyzer calibration report
Repeatability	See analyzer calibration report
Measurement Time ¹	Typically less than 20 seconds
Application Data	
Environmental Temperature Range	-20 °C to 50 °C (-4 °F to 122 °F) - <i>Standard</i> -30 °C to 60 °C (-14 °F to 140 °F) - <i>Optional</i>
Heated Enclosure Temperature	50 ± 5 °C
Shipment and Storage Temperatures	≥ -20 °C (-4 °F)- <i>Standard</i> > 0 °C (32 °F) - <i>Analyzers with perm tube validation</i>
Environmental Relative Humidity	5% to 95%, Non-condensing
Altitude	Up to 2000 m
Sample Cell Operating Pressure Range	800 to 1200 mbar - <i>Standard</i> 950 to 1700 mbar - <i>Optional</i>
Pressure to Cell	70 kPaG (10 PSIG) max to spectrometer cell
Sample Flow Rate	0.5 to 4 SLPM (0.02 to 0.1 SCFM) ¹
Contaminant Sensitivity	None for gas phase glycol, methanol, amines, or mercaptans
Electrical & Communications	
Input Power, Maximum ²	120 or 240 VAC ± 10%, 50 to 60 Hz standard; ~300 W ¹
Communications	<i>Analog:</i> Isolated Analog channels, 1200 ohms at 24 VDC max <i>Outputs:</i> Qty (2) 4 to 20 mA (measurement value) <i>Input:</i> Qty (1) 4 to 20 mA (pipeline pressure) ¹ <i>Serial:</i> Ethernet and RS-485 half-duplex - <i>Standard</i>
Digital Signals	<i>Outputs:</i> (5); Hi/Lo Alarm, General Fault, Validation Fail ¹ , Validation 1 Active ¹ , Validation 2 Active ¹ <i>Inputs:</i> (2); Flow Alarm ¹ , Validation Request ¹
Protocol	Modbus Gould RTU, Daniel RTU or ASCII
Diagnostic Value Examples	Detector Power (Optics Health), Spectrum Reference Comparison and Peak Tracking (Spectrum Quality), Cell Pressure and Temperature (Overall System Health)
LCD Display	Concentration, Cell Pressure, Cell Temperature and Diagnostics

1. Application dependent.

2. Supply voltage not to exceed ± 10% of nominal. Transient over-voltages according to Over-voltage category II.

Table A-1 SS2100i-2 analyzer specifications (Continued)

Physical Specifications	
Electronics Enclosure	IP66 Copper-free Aluminum with Weather-resistant Polyurethane Powder Coating, 80 to 120 micron thickness
Sample System Enclosure(s)	IP55 (min.) 304 or 316L Stainless Steel
Analyzer Dimensions ¹	670 mm H × 1270 mm W × 248 mm D (26.3 in. H × 50 in. W × 9.7 in. D)
Analyzer Weight ¹	Approximately 145 kg (320 lbs) (not including Sample Conditioning System- refer to system drawings)
Sample Cell Construction	316L Series Polished Stainless Steel - <i>Standard</i>
Analyzer Certifications	
Certification ²	CE, ATEX, IECEx:   II 2 G, Ex db IIB+H2 T4 Gb; LCIE 10 ATEX 3108X, IECEx LCI 11.0007X
Analyzer Assembly	 II 2 G, IIB+H2 T3 Gb

1. Dimensions are for analyzer only. Consult system drawings for analyzers with sample conditioning systems.
2. Including an "X" after the certificate number indicates that the product is subject to the Special Conditions of Use specified in the schedule to this certificate. Refer to the Special Conditions of Use under the relevant certification prior to installation or use.



For a complete listing of new or updated certificates for the SS2100i-2 analyzer, please visit the product page at www.endress.com.

Exd Accessory Conditions of Use

All accessories listed in Table A-2 shall comply with the latest IEC/EN 60079-0 and IEC/EN 60079-1 in addition to the conditions listed on the following page.

Table A-2 Exd accessory conditions of use

Accessory Type	Rating	Notes
Stopper Plug	Exd, Zone 1	<ol style="list-style-type: none"> 1. Stopping plugs shall be assembled in such a way that their protrusion from an associated enclosure is not increased. 2. Installer must ensure the stopping plug ingress protection matches the ingress protection rating of the associated enclosure, IP66.

Table A-2 Exd accessory conditions of use (Continued)

Accessory Type	Rating	Notes
Reducer/Adapter	Exd, Zone 1	<ol style="list-style-type: none"> 1. Adapter/reducers shall be assembled in such a way that their protrusion from an associated enclosure is not increased. 2. Installer must ensure the stopping plug ingress matches the ingress protection of the rating of the associated enclosure, IP66. 3. For direct entry Exd applications, only one adapter/reducer shall be used per cable entry. 4. The female connection thread of a Thread Conversion Adapter shall "step" not more than two "size" up in the case of a thread gender change.
Breather/Drainer	Exd, Zone 1	<ol style="list-style-type: none"> 1. The breather/drainer shall be suitable for bottom entry application only. 2. It is the user's responsibility to ensure that the ingress protection level of an associated enclosure is maintained at the interface, IP66. 3. Breather/drainer specified shall meet the following requirements: <ul style="list-style-type: none"> • Exd enclosures with an internal volume $75 \text{ L} \leq V \leq 175 \text{ L}$ • Exd enclosure reference pressure 40 bar maximum.
Cable Gland(s)	Exd, Zone 1	<ol style="list-style-type: none"> 1. Compound Barrier Cable Glands shall be specified for use with our analyzer Exd enclosure. 2. Compound Barrier Cable Glands shall carry a minimum IP66 ingress protection level.

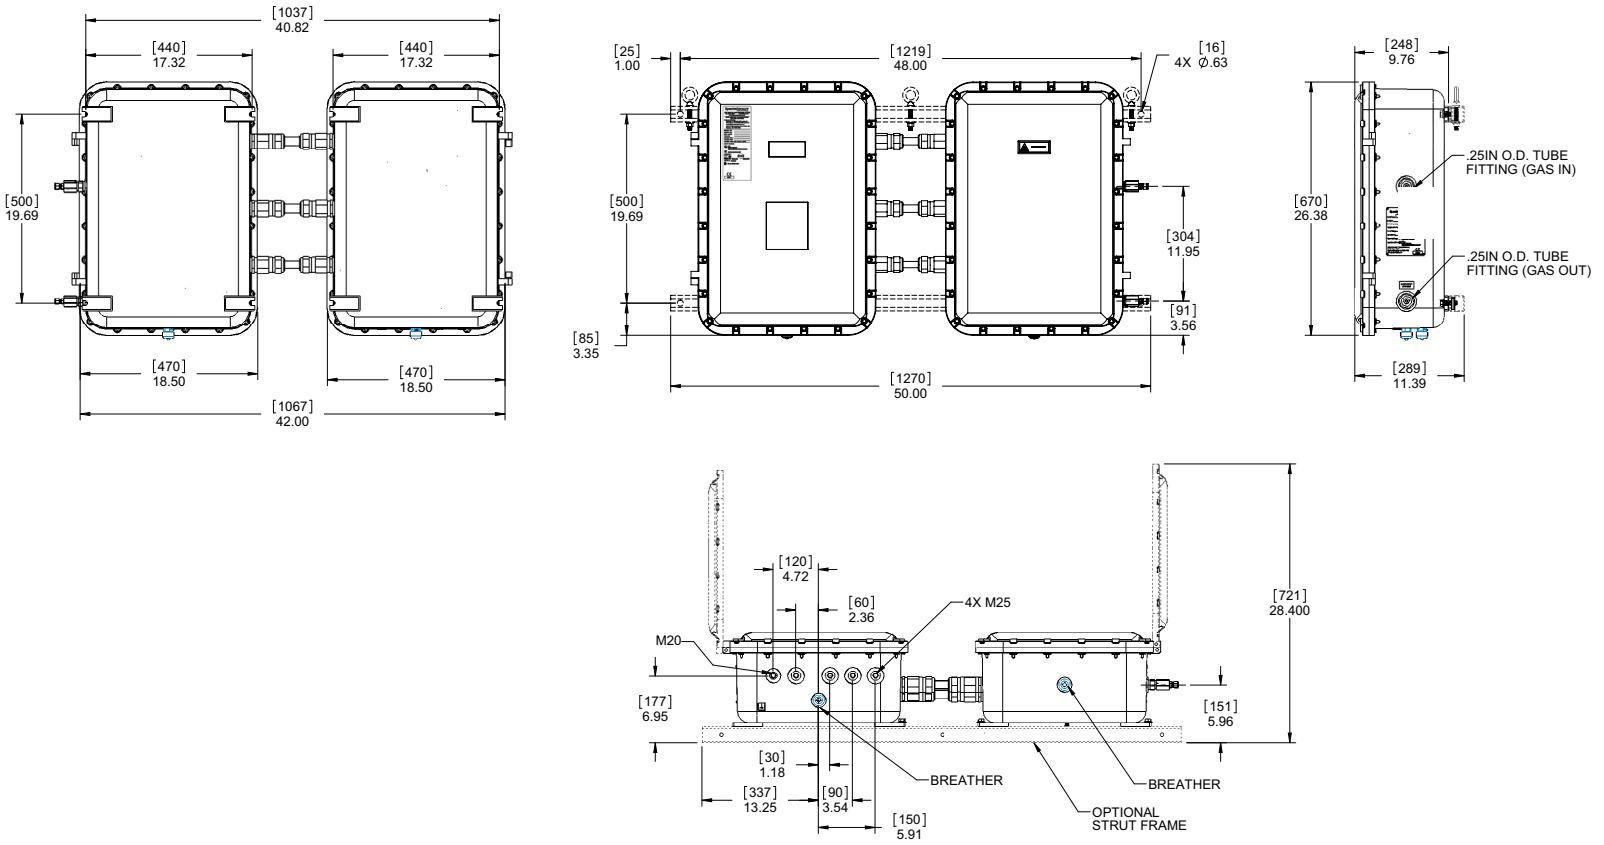


Figure A-1 Dimensions and external components of SS2100i-2 (cable-coupled configuration)

Appendix B: Maintenance & Troubleshooting

CAUTION
CLASS 3B INVISIBLE LASER
RADIATION WHEN OPEN
AVOID EXPOSURE TO THE BEAM

INVISIBLE LASER RADIATION - Avoid exposure to beam. Class 3b Radiation Product. Refer servicing to the manufacturer-qualified personnel.



The optical head has a seal and "WARNING" sticker to prevent inadvertent tampering with the device. Do not attempt to compromise the seal of the optical head assembly. Doing so will result in loss of device sensitivity and inaccurate measurement data. Repairs can then only be performed by the factory and are not covered under warranty.

This section presents recommendations and solutions to common problems, such as gas leaks, excessive sampling gas temperatures and pressures, electrical noise, and contamination. For other issues related to the sample conditioning system (SCS), please refer to the SCS Operating Instruction.

Contact Service if your analyzer does not appear to be hampered by one of these related problems, refer to "**Service Contact**" on page B-30.

Gas Leaks

Probably the most common cause of erroneous measurements is outside air leaking into the sample supply line. It is recommended the supply lines be periodically leak-tested, especially if the analyzer has been relocated or has been replaced or returned to the factory for service and the supply lines have been reconnected.



Do not use plastic tubing of any kind for sample lines. Plastic tubing is permeable to moisture and other substances which can contaminate the sample stream. Endress+Hauser recommends using 1/4 in. O.D. x 0.035 in. wall thickness, seamless stainless steel tubing.



Process samples may contain hazardous material in potentially flammable and/or toxic concentrations. Personnel should have a thorough knowledge and understanding of the physical properties of the sample and prescribed safety precautions before operating the analyzer.

Excessive Sampling Gas Temperatures and Pressures

The embedded software is designed to produce accurate measurements only within the allowable cell operating range, refer to Table A-1 on page A-1.



The cell temperature operating range for analyzers that are equipped with heated enclosures is equal to the enclosure temperature set-point ± 5 °C.

Pressures and temperatures outside this range will trigger a **Pressure Low Alarm**, **Pressure High Alarm**, **Temp Low Alarm**, or **Temp High Alarm** fault. Refer to the Description of Device Parameters for more information on alarms.



If the pressure, temperature, or any other readings on the LCD appear suspect, they should be checked against the specifications, refer to Table A-1 on page A-1.

Electrical Noise

High levels of electrical noise can interfere with laser operation and cause it to become unstable. Always connect the analyzer to a properly grounded power source.

Contamination

Contamination and long exposure to high humidity are valid reasons for periodically cleaning the gas sampling lines. Contamination in the gas sampling lines can potentially find its way to the sample cell and deposit on the optics or interfere with the measurement in some other way. Although the analyzer is designed to withstand some contamination, it is recommended to always keep the sampling lines as contamination free as possible.

To keep the sampling lines clean

1. Make sure that a membrane separator filter (included with most systems) is installed ahead of the analyzer and operating normally. Replace the membrane if necessary. If liquid enters the cell and accumulates on the internal optics, a **Laser Power Low Alarm** fault will result.
2. If mirror contamination is suspected, see **"To clean the mirror"** on page B-5.

3. Turn off the sample valve at the tap in accordance with site lock-out, tag-out rules.
4. Disconnect the gas sampling line from the sample supply port of the analyzer.
5. Wash the sampling line with alcohol or acetone and blow dry with mild pressure from a dry air or nitrogen source.
6. Once the sampling line is completely free of solvent, reconnect the gas sampling line to the sample supply port of the analyzer.
7. Check all connections for gas leaks. Endress+Hauser recommends using a liquid leak detector.

Mirror contamination

If contamination makes its way into the cell and accumulates on the internal optics, a **Laser Power Low Alarm** fault will result.

Cleaning the Mirrors

If mirror contamination is suspected in your SS2100i-2, contact Service before attempting to clean the mirrors. Refer to "**Service Contact**" on page B-30. If advised to do so, use the following procedure.



*This procedure should be used ONLY when necessary and is not part of routine maintenance. Refer to "**Service Contact**" on page B-30 before cleaning mirrors to avoid compromising the system warranty.*

CAUTION
CLASS 3B INVISIBLE LASER
RADIATION WHEN OPEN
AVOID EXPOSURE TO THE BEAM

INVISIBLE LASER RADIATION - Avoid exposure to beam. Class 3b Radiation Product. Refer servicing to the manufacturer-qualified personnel.

Tools and supplies

- Lens cleaning cloth (Cole Parmer® EW-33677-00 TEXWIPE® Alphawipe® Low-Particulate Clean Room Wipes or equivalent)
- Reagent-grade isopropyl alcohol (ColeParmer® EW-88361-80 or equivalent)



Alcohol can be hazardous. Follow all safety precautions when in use and thoroughly wash hands prior to eating.

- Small drop dispenser bottle (Nalgene® 2414 FEP Drop Dispenser Bottle or equivalent)
- Hemostat (Fisherbrand™ 13-812-24 Rochester-Pean Serrated Forceps)
- Bulb blower or dry compressed air/nitrogen
- O-rings (refer to Table C-7 on page C-17 for specific part number)
- Torque wrench
- Permanent ink marker
- Non-outgassing grease
- Flashlight

Determining the type of cell mirror

Measurement cells will come equipped with either a glass or stainless steel mirror. Before determining whether to clean or replace the mirror, identify the type of measurement cell being used in the analyzer. Refer to Figure B-1 below.


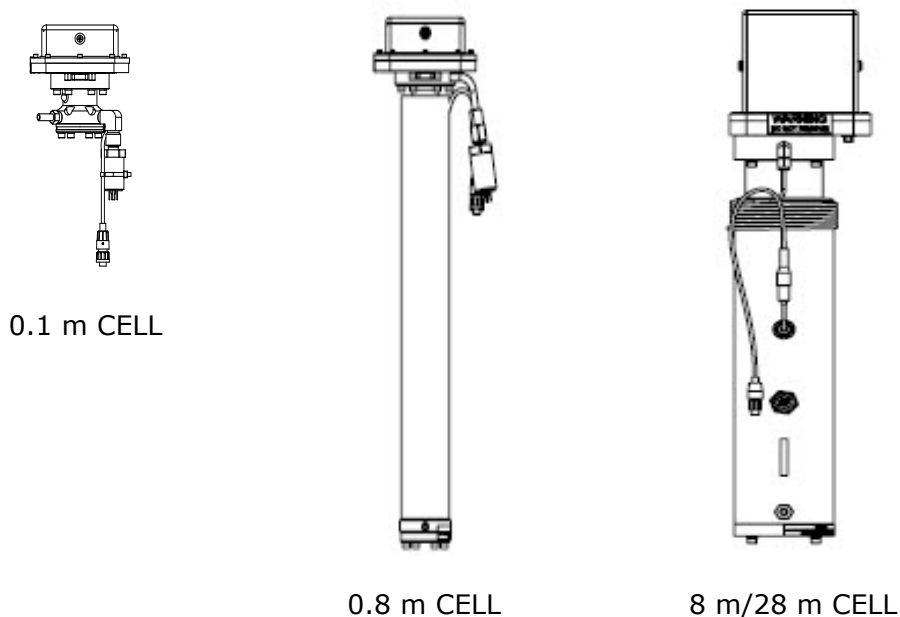


Figure B-1 Measurement cell types

The stainless steel mirrors are used with 0.1 m and 0.8 m measurement cells only. The stainless steel mirrors have been identified with either an "X" engraved on the outside bottom of the mirror or a groove around the rim of the mirror. Glass mirrors can be used on any size cell. To determine the type of mirror being used for the system cell, follow the steps below.

1. Feel at the bottom of the cell for the engraved "X" marking or the side of the mirror for a groove. Refer to Figure B-2.

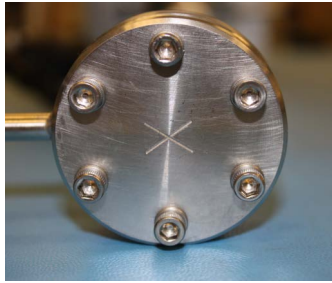

MIRROR MARKED
WITH 'X'



MIRROR GROOVED
RIM - SIDE VIEW

Figure B-2 Stainless steel mirror marking

- a. If the bottom surface is smooth, a glass mirror is being used.
- b. If the bottom surface is rough or engraved, or a groove on the side of the mirror is detected, a stainless steel mirror is being used.



Only the stainless steel mirror can be replaced. A glass mirror cannot be replaced. Do not attempt to replace a glass mirror with a stainless steel mirror or system calibration may be adversely affected. A stainless mirror may only be replaced with a stainless steel mirror.

To clean the mirror, refer to the instructions **"To clean the mirror"** on page B-5. To replace a stainless steel mirror, refer to the instructions for **"To replace the stainless steel mirror"** on page B-7.

To clean the mirror

To clean either the glass or stainless steel mirror, use the following procedure.

1. Power down the analyzer following the procedure outlined in the appropriate chapter in the Description of Device Parameters for your analyzer under **"Powering Down the Analyzer"**.
2. Disconnect the sample supply and return tubes from the analyzer.



All valves, regulators, switches, etc. should be operated in accordance with site lock-out/tag-out procedures.

3. If possible, purge the system with nitrogen for 10 minutes.



Process samples may contain hazardous material in potentially flammable and/or toxic concentrations. Personnel should have a thorough knowledge and understanding of the physical properties of the sample and prescribed safety precautions before operating the analyzer.

4. Carefully mark the orientation of the mirror assembly on the cell body.



Careful marking of the mirror orientation is critical to restoring system performance upon reassembly after cleaning.

5. Gently remove the mirror assembly from the cell by removing the socket-head cap screws and set on a clean, stable and flat surface.



The sample cell assembly contains a low-power, 10 mW MAX, CW Class 3b invisible laser with a wavelength between 750 to 3000 nm. Never open the sample cell flanges or the optical assembly unless the power is turned off.



Always handle the optical assembly by the edge of the mount. Never touch the coated surfaces of the mirror.

6. For the 28 m and 8 m cells, look inside the sample cell at the top mirror using a flashlight to ensure that there is no contamination on the top mirror. For 0.8 m cells, skip and proceed to the next step.



*Endress+Hauser does not recommend cleaning the top mirror. Refer to "**Service Contact**" on page B-30 to contact Service if the top mirror is visibly contaminated.*

7. Remove dust and other large particles of debris from the lower mirror using a bulb blower or dry compressed air/nitrogen.



Pressurized gas duster products are not recommended as the propellant may deposit liquid droplets onto the optic surface.

8. Put on clean acetone-impenetrable gloves.
9. Double-fold a clean sheet of lens cleaning cloth and clamp near and along the fold with the hemostats or fingers to form a "brush."

10. Place a few drops of isopropyl alcohol onto the mirror and rotate the mirror to spread the liquid evenly across the mirror surface.
11. With gentle, uniform pressure, wipe the mirror from one edge to the other with the cleaning cloth only once and only in one direction to remove the contamination. Discard the cloth.



Never rub an optical surface, especially with dry tissues, as this can mar or scratch the coated surface.

12. Repeat with a clean sheet of lens cleaning cloth to remove the streak left by the first wipe. Repeat, if necessary, until there is no visible contamination on the mirror.
13. Replace the O-ring adding a very thin layer of grease and ensuring it is properly seated.
14. Carefully replace the mirror assembly onto the cell in the same orientation as previously marked.
15. Tighten the socket-head cap screws evenly with a torque wrench to 30 in-lbs (28 m or 8 m sample cell) or 13 in-lbs (0.8 m sample cell).

To replace the stainless steel mirror

If your system has been configured with a stainless steel mirror (0.1 m/0.8 m measurement cells only), use the following instructions for replacing the mirror.



*Refer to "**Service Contact**" on page B-30 if a glass mirror requires replacement. Do not attempt to replace a glass mirror with a stainless steel mirror or system calibration may be adversely affected.*

1. Power down the analyzer following the procedure outlined in the appropriate chapter in the Description of Device Parameters for your analyzer under "**Powering Down the Analyzer**".
2. Disconnect the sample supply and return tubes from the analyzer.



All valves, regulators, switches, etc. should be operated in accordance with site lock-out/tag-out procedures.

3. If possible, purge the system with nitrogen for 10 minutes.



Process samples may contain hazardous material in potentially flammable and/or toxic concentrations. Personnel should have a thorough knowledge and understanding of the physical properties of the sample and prescribed safety precautions before operating the analyzer.

4. Gently remove the mirror assembly from the cell by removing the six socket-head cap screws and set on a clean, stable and flat surface.



Always handle the optical assembly by the edge of the mount. Never touch the surface of the mirror.



*Endress+Hauser does not recommend cleaning the top mirror. Refer to "**Service Contact**" on page B-30 to contact Service if the top mirror is visibly contaminated.*

5. After the mirror has been removed, confirm the need to replace mirror due to contamination. If yes, set mirror aside.
6. Put on clean acetone-impenetrable gloves.
7. Obtain the new stainless steel mirror. Refer to Figure B-3.

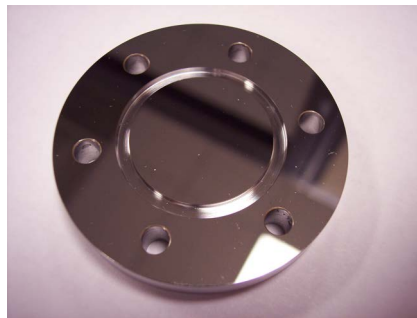


Figure B-3 *Stainless steel mirror — mirror side up*

8. Check the O-ring.
 - a. If a new O-ring is needed, apply grease on fingertips and then to the new O-ring.
 - b. Place newly greased O-ring into the groove around the outside of the mirror taking care not to touch the mirror surface.
9. Carefully place the new stainless steel mirror onto the cell making sure the O-ring is properly seated.
10. Tighten the socket-head cap screws evenly with a torque wrench to 13 in-lbs.

Pressure Sensor Replacement

A pressure sensor may need to be replaced in the field as a result of one or more of the following conditions:

- Loss of pressure reading
- Incorrect pressure reading
- Pressure sensor not responding to pressure change
- Physical damage to the pressure sensor

Replacing the pressure sensor on a 8 m/28 m cell

Use the following instruction to replace a pressure sensor on a 8 m/28 m measurement cell.

Tools and supplies

- Acetone-impenetrable gloves (North NOR CE412W Nitrile Chemsoft™ CE Cleanroom Gloves or equivalent)
- 9/16 in. wrench
- 7/8 in. wrench
- 9/64 in. hex key
- Flat-head screwdriver
- Phillips-head screwdriver
- Metal pick
- Military grade stainless steel PTFE tape (or equivalent)
- Dry nitrogen
- Isopropyl alcohol



Alcohol can be hazardous. Follow all safety precautions when in use and thoroughly wash hands prior to eating.

To replace the pressure sensor on a 8 m/28 m cell

1. Close the external flow of gas at the sample inlet.
2. Purge the system by connecting dry nitrogen to the sample inlet. Allow the SCS to purge for 5 to 10 minutes.
3. Close the nitrogen flow.
4. Power off the system. Refer to the Description of Device Parameters for this analyzer for "**Powering down the analyzer**".

5. Open the door to the measurement cell enclosure. Refer to Figure B-4.

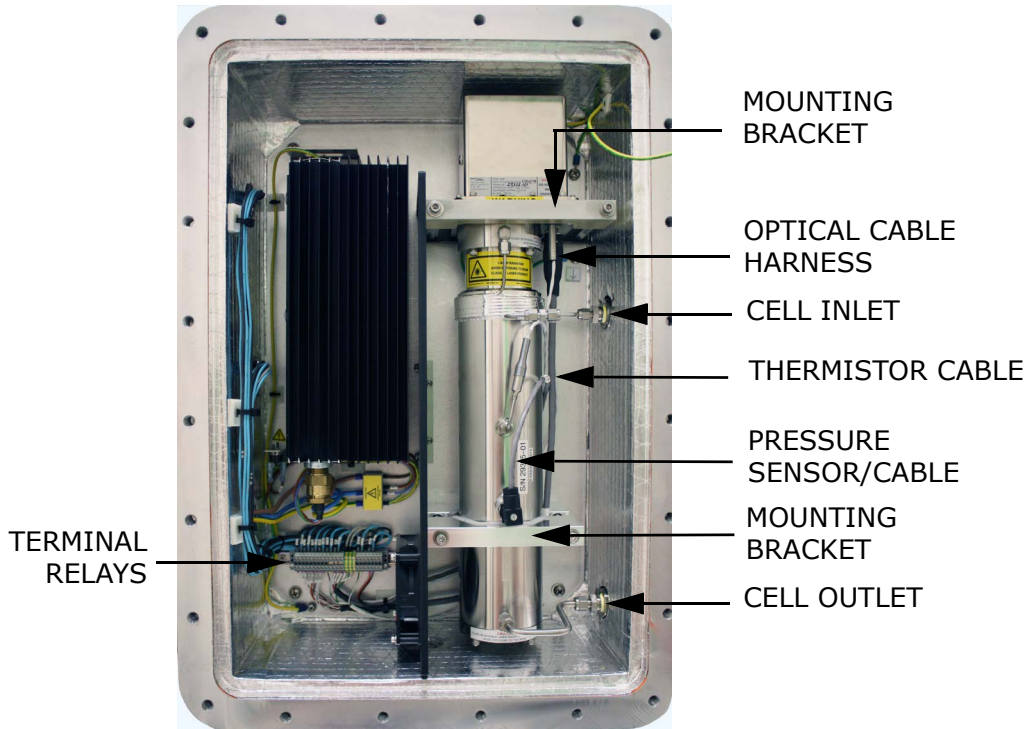


Figure B-4 Cell cabinet interior

6. Remove the optical cable harness using a flat-head screwdriver.
7. Disconnect the cell inlet using a 9/16 in. wrench.
8. Disconnect the cell outlet using a 9/16 in. wrench.
9. Disconnect the thermistor cable at the circular connector.
10. Remove the pressure sensor cable from the circular connector inside the enclosure.

For new model pressure sensors with quick-disconnects, detach the pressure sensor cable from the pressure sensor at the connector using a Phillips-head screwdriver. Do not remove the black connector from the cable inside the enclosure. Dismount the cell from the bracket by removing the four securing screws (two on top, two on the bottom) using a 9-64 in. Hex Key. Place the measurement cell on a clean, flat surface with the pressure sensor facing up. Refer to Figure B-5 on page B-11.



Figure B-5 Removed 28 m measurement cell



Orient the measurement cell to avoid any debris from entering the cell.

- 11.** Holding the cell firmly with one hand, use a 7/8 in. wrench to remove the old (to be replaced) pressure sensor as shown in Figure B-6 below.

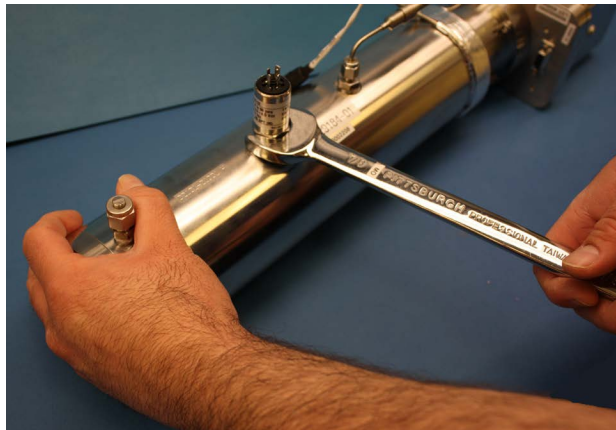


Figure B-6 Removing the old pressure sensor

- a.** Turn the 7/8 in. wrench counterclockwise to loosen the pressure sensor until it is able to be removed.
- 12.** Remove excess seal tape from the threads at the opening and check for galling. Refer to Figure B-7 on page B-12.



Figure B-7 Removing excess seal tape from flange



Tip the measurement cell forward so that any loose debris falls to the flat surface and not back inside the cell.



*Threads showing signs of galling indicate a possible leak. Contact Service to arrange for repair, refer to "**Service Contact**" on page B-30.*

- 13.** If you suspect debris has fallen into the measurement cell, refer to "**Cleaning the Mirrors**" on page B-3 to check for any debris.
- 14.** Check for tape fragments inside the cell and remove with a swab. Refer to Figure B-8.



Figure B-8 Removing excess seal tape from inside cell

15. Remove the new pressure sensor from the packaging. Retain the black connector cap on the sensor - do not remove.
16. Wrap stainless steel PTFE tape around the threads at the top of the pressure sensor, beginning from the base of the threads to the top, approximately three times taking care to avoid covering the top opening. Refer to Figure B-9.



Figure B-9 Replacing seal tape

18. Holding the cell steady, insert the new pressure sensor into the threaded opening. Refer to Figure B-10.



Figure B-10 Replacing pressure sensor

19. Hand tighten the pressure sensor clockwise into the opening until no longer moving freely.
20. Holding the cell in place, turn the sensor clockwise with a 7/8 in. wrench until tight. Two or three threads on the pressure sensor should still be visible.



Make sure the black connector at the end of the pressure sensor is facing towards the head or the base of the measurement cell to facilitate connection. Refer to Figure B-11 on page B-14.



Figure B-11 New pressure sensor installed

21. Remove the black connector from the pressure sensor and discard.



If a new cable is required, connect the new harness/cable to the new pressure sensor at this point.

22. Remount the cell to the mounting brackets using a 9/64 in. Hex Key with the pressure sensor facing out towards the cabinet door.
23. Reinstall cell inlet and cell outlet using a 9/16 in. wrench.
24. Reconnect the thermistor connector.
25. Connect the new pressure sensor harness to the existing cable at the black connector.
26. Reconnect the optical cable harness.
27. Close the analyzer enclosure cover.
28. Conduct a leak test to determine that the new pressure sensor is not leaking.



Do not allow cell to exceed 10 PSIG or damage could occur.



*Contact Service for any questions related to leak testing the pressure sensor, refer to "**Service Contact**" on page B-30.*

29. Turn the system power on. Refer to the Description of Device Parameters for this analyzer for "**Powering up the analyzer.**"

30. Run a validation on the analyzer. Refer to the Description of Device Parameters for instructions on **"Validating the Analyzer."**
 - a. If the system passes, the pressure sensor replacement is successful.
 - b. If the system does not pass, refer **"Service Contact"** on page B-30 for instruction.

Replacing the pressure sensor on a 0.8 m cell

Use the following instruction to replace a pressure sensor on a 0.8 m measurement cell.

Tools and supplies

All tools and materials listed in **"Replacing the pressure sensor on a 8 m/28 m cell"** on page B-9 will be necessary to complete this instruction with the exception of the following:

- Acetone-impenetrable gloves (North NOR CE412W Nitrile Chemsoft™ CE Cleanroom Gloves or equivalent)

To replace the pressure sensor on a 0.8 m cell

Follow steps 1-10 listed under **"To replace the pressure sensor on a 8 m/28 m cell"** on page B-9. Continue with the following steps.

1. Dismount the cell from the bracket by removing the four securing screws (two on top, two on the bottom) using a 9/64 in. hex key. Place the measurement cell on a clean, flat surface with the pressure sensor facing up. Refer to Figure B-12.

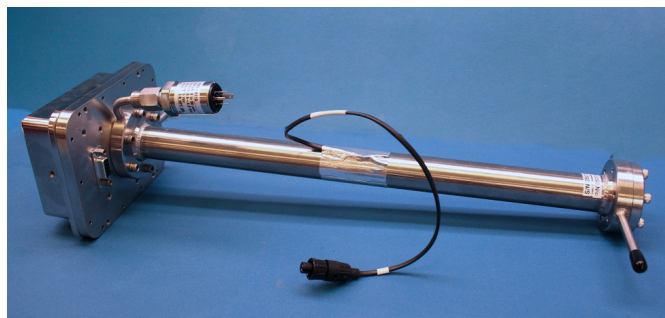


Figure B-12 Removed 0.8 m measurement cell with pressure sensor face up



Orient the measurement cell to avoid any debris from entering the cell.

2. Using a 9/16 in. wrench, secure the flange while using a 7/8 in. wrench to remove the old pressure sensor. Refer to Figure B-13.

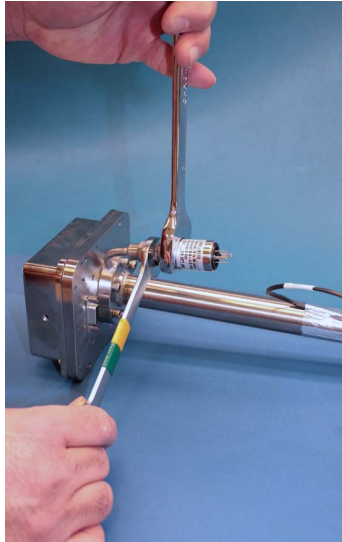


Figure B-13 Removing the old pressure sensor

- a. Hold the wrench on the flange stable and parallel to the surface. Do not move.
 - b. Turn the 7/8 in. wrench counterclockwise to loosen the pressure sensor until it is able to be removed.
3. Remove excess seal tape from the flange opening and threads and check threads for galling. Refer to Figure B-14.

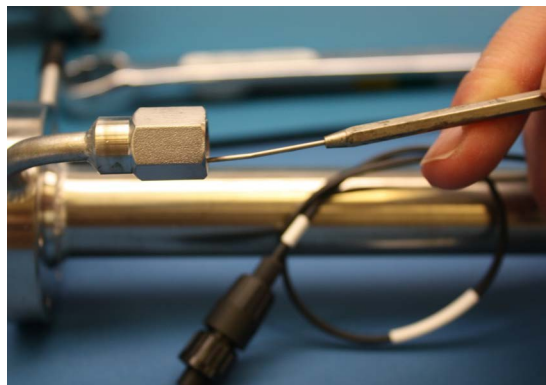


Figure B-14 Removing excess seal tape from flange



Threads showing signs of galling indicate a possible leak. Contact Service to arrange for repair, refer to "**Service Contact**" on page B-30.

4. Remove the new pressure sensor from the packaging. Retain the black connector cap on the sensor - do not remove.
5. Wrap stainless steel PTFE tape around the threads at the top of the pressure sensor, beginning from the base of the threads to the top, approximately three times taking care to avoid covering the top opening. Refer to Figure B-15.



Figure B-15 Replacing seal tape

6. Insert the new pressure sensor into the threaded flange keeping the sensor parallel to the surface for proper fitting.
7. Hand tighten the pressure sensor turning it clockwise into the flange until no longer moving freely. Refer to Figure B-16.

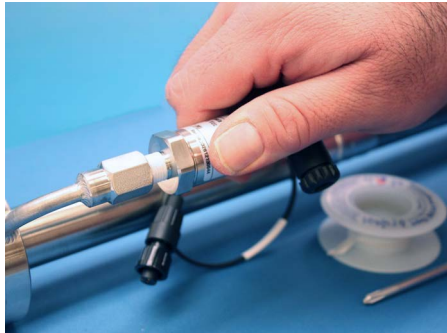


Figure B-16 Replacing pressure sensor

8. Using the 9/16 in. wrench to hold the flange in place, turn the sensor clockwise with a 7/8 in. wrench until tight. Two or three threads on the pressure sensor should still be visible.



Make sure the black connector at the bottom of the pressure sensor is facing up from the measurement cell. Refer to Figure B-17 on page B-18.



Figure B-17 Newly installed pressure sensor positioning

9. Remove the black connector from the pressure sensor and discard.



If a new cable is required, connect the new harness/cable to the new pressure sensor at this point.

10. Remount the cell to the mounting brackets using a 9/64 in. Hex Key with the pressure sensor facing forward.
11. Reinstall cell inlet and cell outlet using a 9/16 in. wrench.
12. Reconnect the thermistor.
13. Reconnect the new pressure sensor harness to the existing cable at the black connector, or connect the new pressure sensor harness and cable to the circular connector, as applicable.
14. Reconnect the optical cable harness.
15. Close the analyzer enclosure cover.
16. Conduct a leak test to determine that the new pressure sensor is not leaking.



Do not allow cell to exceed 10 PSIG or damage could occur.



*Contact Service for any questions related to leak testing the pressure sensor, refer to "**Service Contact**" on page B-30.*

17. Turn the system power on. Refer to the Description of Device Parameters for this analyzer for "**Powering up the analyzer**".

18. Run a validation on the analyzer. Refer to the Description of Device Parameters for instructions on **"Validating the Analyzer."**
 - a. If the system passes, the pressure sensor replacement is successful.
 - b. If the system does not pass, contact Service, refer to **"Service Contact"** on page B-30.

Replacing the dryer

1. Shut off the gas flow (purge the analyzer, depending on gas stream being used).
2. Open the SCS enclosure door.
3. Using a wrench, loosen the female fitting at the top and bottom of the dryer. Refer to Figure B-18.

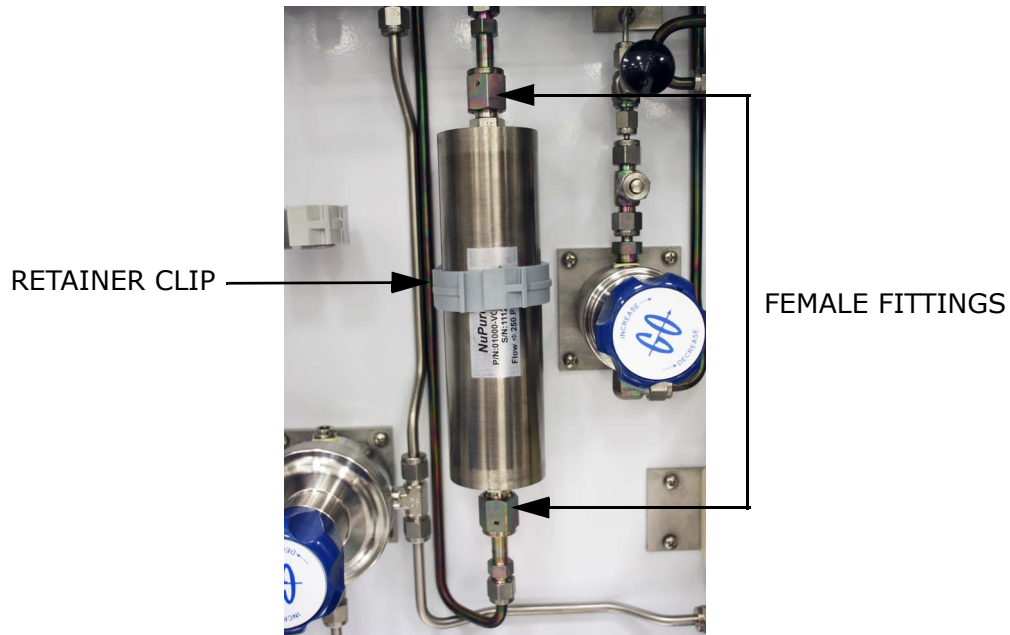


Figure B-18 Installed dryer



The VCR metal gasket face seal fitting is currently used on low moisture systems only.

4. Open the retainer clip by grasping each side and squeezing towards the middle. Carefully release the retainer clip by inserting a tool (e.g., screwdriver) while squeezing.

5. Remove the dryer.
6. Insert the new dryer into the analyzer.
7. Re-fasten the retainer clip gasket onto the new dryer unit.



Refer to your analyzer's spare parts list or contact Service for ordering assistance. For Service, refer to "**Service Contact**" on page B-30.

8. Connect the female nuts at the top and bottom of the dryer to finger tight.
9. Using a wrench, tighten the female nuts 1/8 turn from finger tight.
10. Close the SCS enclosure door.
11. Turn on gas flow to the analyzer.
12. Perform a leak test.



Contact Service for any questions related to leak testing, refer to "**Service Contact**" on page B-30.

Flame Arrestor Replacement and Safety

The analyzer system comes equipped with a protective covering over the flame arrestors and tubing that runs from the analyzer electronics to the SCS. Refer to the analyzer system drawings to locate the protective enclosure for your analyzer; the location of which can vary by customer configuration.

Tools Required

- 7/16 in. angle double open-end wrench
- 9/16 in. angle double open-end wrench
- 7/8 in. wrench

To replace the flame arrestors

1. Ensure all safety requirements have been met and any necessary protective gear and tools are being used.



Refer to "**Potential health effects**" on page B-22 before removing insulation.

2. Purge the system following the instructions provided in steps 1 through 8 in **"Preparing the analyzer for shipment or storage"** on page B-30.
3. Remove the screws holding the protective cover in place and lift up on the cover to remove from the enclosure.
4. Remove the insulation packed inside the enclosure and place in a clean, dry area. Refer to Figure B-19.



Figure B-19 Unpacking enclosure insulation

5. Disassemble the tubing using a 9/16 in. wrench. Refer to Figure B-20.

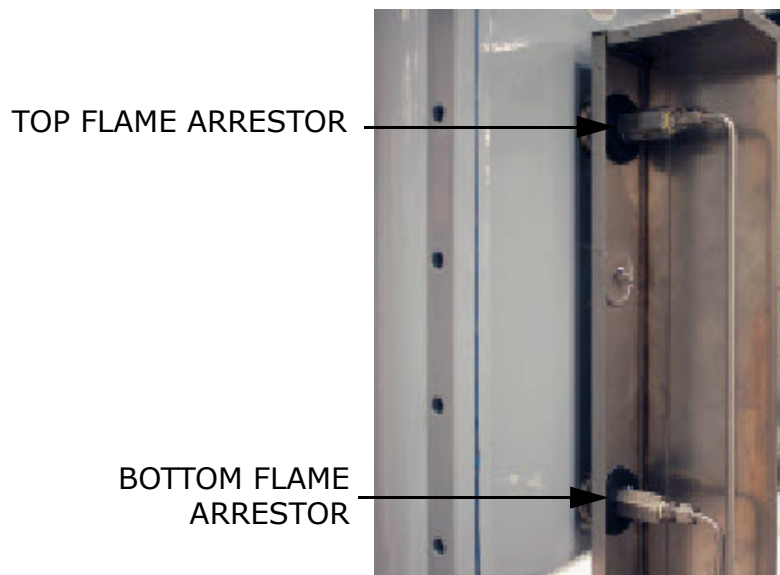


Figure B-20 Flame arrestor positions inside the enclosure

6. Remove the flame arrestor using a 7/8 in. wrench. Refer to Figure B-21.
 - a. After the seal is broken, the flame arrestor may be loosened by hand and removed.

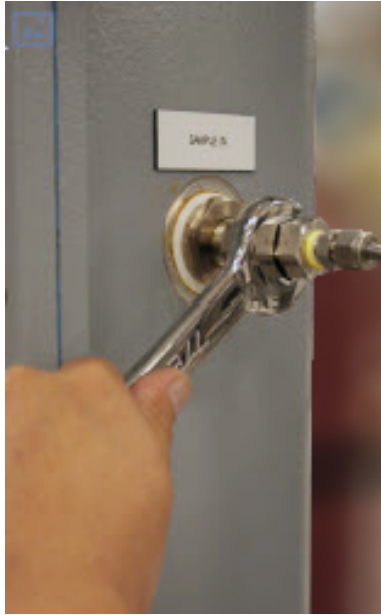


Figure B-21 Removing the flame arrestor

7. Insert the new flame arrestor ensuring its proper seating inside the washer.
8. Tighten the flame arrestor by hand turning clockwise. Use the hook spanner wrench to fully tighten.
9. Reassemble SCS tubing and conduct a leak test.
10. Repack the insulation into the enclosure and replace the cover.
11. Replace screws to secure the enclosure cover.

Potential health effects

The flame arrestor enclosure is packed with insulation material that can cause health issues if inhaled, exposed to bare skin or in direct contact with eyes. Please follow the safety procedures for unpacking this enclosure to access the

flame arrestors and review the following potential health effects of the insulation material before beginning maintenance on the flame arrestors.



- Eyes: Direct contact with eye can cause mechanical irritation.
- Skin: The material (when in wet state or as a dust) is not chemically harmful if it comes in contact with the skin and is not immediately washed off. However, direct contact of dust and mineral wool fibers with skin can cause skin irritation (mechanical) and itchiness.
- Ingestion: No known effects.
- Inhalation: Inhalation of dust can cause nose, throat, lungs and upper respiratory tract irritation. Persons exposed to dust may be forced to leave area because of nuisance conditions such as coughing, sneezing and nasal irritation.
- Chronic: Persons with chronic or systemic skin or eye disease should use precautions and wear all personal protective equipment when working with this product.

Transport Information

U.S. DOT Information: Not a hazardous material per DOT shipping requirements. Not classified or regulated.

Regulatory Information

Canadian Regulations

- WHMIS: D2B
All components of this product are included in the Canadian Domestic Substances List (DSL) or the Canadian Non-Domestic Substances List (NDSL).

USA Regulations

- All ingredients of this product are included in the U.S. Environmental Protection Agency's Toxic Substances Control Act Chemical Substance Inventory.

Table B-1 Carcinogenicity Classification of Ingredients

Material	IARC	NTP
Man Made Vitreous Fiber	Group 3	None

In October 2001, the International Agency for Research on Cancer (IARC) classified mineral wool fibers (rock or slag) as Group 3 (not classifiable as to carcinogenicity to humans). IARC noted specifically: "no evidence of increased risks of lung cancer or mesothelioma (cancer of the lining of the body cavities) from occupational exposures during manufacture of these materials, and inadequate evidence overall of any cancer risk." this was a reversal of the IARC finding in 1987 of a Group 2B designation (possibly carcinogenic to humans) based on earlier studies in which animals were injected with large quantities of slag wool fibers.

Other information**Table B-2** Information for Handling and Identification of Chemical Hazards

Condition	NFPA Ratings	HMIS Ratings	Personal Protection
Health	0	0	Use eye and skin protection. Use NIOSH/MSHA-approved respiratory protection when necessary.
Fire	0	0	
Reactivity	0	0	
Other	N/A		

Legend:

- 0 = Minimal hazard
- 1 = Slight hazard
- 2 = Moderate hazard
- 3 = Serious hazard
- 4 = Severe hazard

Peak Tracking Reset Procedure

The analyzer's software is equipped with a peak tracking function that keeps the laser scan centered on the absorption peak. Under some circumstances, the peak tracking function can get lost and lock onto the wrong peak. If the **PeakTk Restart Alarm** is displayed, the peak tracking function should be reset. Refer to the Description of Device Parameters for this analyzer for instruction.

Instrument Issues

If the instrument does not appear to be hampered by gas leaks, contamination, excessive sampling gas temperatures and pressures, or electrical noise, refer to Table B-3 before contacting Service. Refer to "**Service Contact**" on page B-30.

Table B-3 Potential instrument problems and their solutions

Symptom	Response
Non-Operation (at/after start up)	Is the power connected to both the analyzer and power source? Is the switch on?
	Is the power source good? (100-250 VAC at 50-60 Hz, 9-16 VDC, 18-32 VDC).
	Check fuse(s). If bad, replace with equivalent fuse.

Non-Operation (at/after start up) (continued)	Contact Service for more information, refer to " Service Contact " on page B-30.
Laser Power Low Alarm	Turn off the power to the unit and check the optical head cables for a loose connection. Do not disconnect or reconnect any optical head cables with the power connected.
	Check the inlet and outlet tubes to see if they are under any stress. Remove the connections to the inlet and outlet tubes and see if the power goes up. Perhaps the existing tubing needs to be replaced with stainless steel flexible tubing.
	Refer to the Description of Device Parameters for your analyzer for instructions to capture diagnostic data and submit to Endress+Hauser.
	Possible alignment problem. Contact Service for more information, refer to " Service Contact " on page B-30.
Power Fail	Refer to the Description of Device Parameters for your analyzer for instruction.
	Refer to the Description of Device Parameters for your analyzer for instructions to capture diagnostic data and submit to Endress+Hauser, refer to " Service Contact " on page B-30.
Null Fail	Refer to the Description of Device Parameters for your analyzer for instruction.
	Refer to the Description of Device Parameters for your analyzer for instructions to capture diagnostic data and submit to Endress+Hauser, refer to " Service Contact " on page B-30.

Table B-3 Potential instrument problems and their solutions (Continued)

Symptom	Response
Spectrum Fail	Reset the Peak Tracking function. Refer to the Description of Device Parameters for your analyzer for instruction.
	Refer to the Description of Device Parameters for your analyzer for instructions to capture diagnostic data and submit to Endress+Hauser, refer to " Service Contact " on page B-30.
Track Fail	Refer to the Description of Device Parameters for your analyzer for instruction.
	Reset the Peak Tracking function. Refer to the Description of Device Parameters for your analyzer for instruction.
Pressure Low Alarm or Pressure High Alarm	Check that the actual pressure in the sample cell is within specification (Table A-1 on page A-1).
	If the pressure reading is incorrect, check that the pressure/temperature cable on the bottom of the electronics enclosure is tight. Check the connector on the pressure sensor. Check the pressure connector on the backplane board.
Temp Low Alarm or Temp High Alarm	Check that the actual temperature in the sample cell is within specification (Table A-1 on page A-1). For systems with a heated enclosure, check that the temperature in the sample cell is within ± 5 °C of the specified enclosure temperature.
	If the temperature reading is incorrect, check that the pressure/temperature cable on the bottom of the electronics enclosure is tight. Check the connector on the cell temperature sensor. Check the temperature connector on the backplane board. (Note: A temperature reading greater than 150 °C indicates a short circuit on the temperature sensor leads; a reading of less than -40 °C indicates an open circuit).

Table B-3 Potential instrument problems and their solutions (Continued)

Symptom	Response
System stuck in Fit Delta Exceeds Limit restart for greater than 30 minutes	Contact Service for information, refer to " Service Contact " on page B-30.
Not getting enough flow to the sample cell	Check both the micro filter and membrane separator for contamination. Replace if necessary. Refer to the Sample Conditioning System (SCS) Operating Instruction for instruction.
	Check if supply pressure is sufficient.
No reading on device connected to current loop	Make sure that connected device can accept a 4 to 20 mA signal. The analyzer is set to source current.
	Make sure the device is connected to the correct terminals (see Figure 3-3 on page 3-8).
	Check the open circuit voltage (35 to 40 VDC) across the current loops terminals (see Figure 3-3 on page 3-8).
	Replace the current loop device with a milliamperemeter and look for current between 4 mA and 20 mA. A voltmeter connected across a 249 ohm resistor can be used instead of the milliamperemeter; it should read between 1 and 5 volts.
Current loop is stuck at 4 mA or 20 mA	Check display for error message. If alarm has been triggered, reset the alarm.
	On the current loop board, check the voltage between the end of resistor R1 closest to the jumper and ground. If the concentration reading is high, the voltage should be near 1 VDC. If the concentration reading is low, the voltage should be near 4.7 VDC. If not, the problem is probably on the ARM9 main board. Return to factory for service, refer to " Service Contact " on page B-30.

Table B-3 Potential instrument problems and their solutions (Continued)

Symptom	Response
Front panel display is not lit and no characters appear	Check for correct voltage on terminal block input. Observe polarity on DC powered units.
	Check for correct voltage after fuses.
	Check for 5 VDC on red wires, 12 VDC on yellow wires, and 24 VDC on orange wires from power supply.
	Check connections on display communication and power cables.
Strange characters appear on front panel display	Check connections on display communication cable.
Pressing keys on front panel do not have specified effect	Check connections on keypad cable.
Reading seems to always be high by a fixed amount	Capture diagnostic data and send the file to Endress+Hauser (refer to the section called "To read diagnostic data with HyperTerminal" in the firmware communications chapter for your analyzer's firmware version).
Reading seems to always be high by a fixed percentage	Capture diagnostic data and send the file to Endress+Hauser (refer to the section called "To read diagnostic data with HyperTerminal" in the firmware communications chapter for your analyzer's firmware version).
Reading is erratic or seems incorrect	Check for contamination in the sample system, especially if the readings are much higher than expected.
	Capture diagnostic data and send the file to Endress+Hauser (refer to the section called "To read diagnostic data with HyperTerminal" in the firmware communications chapter for your analyzer's firmware version).

Table B-3 Potential instrument problems and their solutions (Continued)

Symptom	Response
Reading displays 0.0 or seems relatively low	Capture diagnostic data and send the file to Endress+Hauser (refer to the section called "To read diagnostic data with HyperTerminal" in the firmware communications chapter for your analyzer's firmware version).
	Check that Peak Tracking is enabled (refer to the section called "To change parameters in Mode 2" in the firmware operations chapter for your analyzer's firmware version).
Reading goes to '0'	If 4 to 20 mA Alarm Action is set to 1 , look on display for an error message (refer to the section called "To change parameters in Mode 2" in the firmware operations chapter for your analyzer's firmware version).
	Gas concentration is equal to zero.
Reading goes to full scale	If 4 to 20 mA Alarm Action is set to 2 , look on display for an error message (refer to the section called "To change parameters in Mode 2" in the firmware operations chapter for your analyzer's firmware version).
	Gas concentration is greater than or equal to full scale value.
Serial output is displaying garbled or no data	Make sure the computer COM port is set for 9600 baud, 8 data bits, 1 stop bit, no parity, and no flow control.
	Be sure no other programs are using the COM port selected.
	Make sure the connections are good. Verify the correct pin connections with an ohm meter.
	Make sure to select the correct COM port into which the cable is plugged.
LCD does not update. Unit is locked up for more than 5 minutes.	Switch off power, wait 30 seconds, and then switch power back on.

Service Contact

For Service, refer to our website for the list of local sales channels in your area (www.endress.com).

Service Repair Order

If returning the unit is required, obtain a **Service Repair Order (SRO) Number** from Service before returning the analyzer to the factory. Your service representative can determine whether the analyzer can be serviced on site or should be returned to the factory. All returns should be shipped to:

Endress+Hauser
11027 Arrow Route
Rancho Cucamonga, CA 91730
United States
www.endress.com

Packing, Shipping and Storage

Endress+Hauser analyzer systems and auxiliary equipment are shipped from the factory in appropriate packaging. The SS2100i-2 analyzer is typically packed in a wooden crate. All inlets and vents are capped and protected when packaged for shipment.

If the equipment is to be shipped immediately or stored for any length of time, it should be packed in the original packaging when shipped from the factory. If analyzer has been installed and or operated (even for purposes of a demonstration), the system should first be decontaminated (purged with an inert gas) before powering down the analyzer.



Process samples may contain hazardous material in potentially flammable and/or toxic concentrations. Personnel should have a thorough knowledge and understanding of the physical properties of the sample and prescribed safety precautions before installing, operating or maintaining the analyzer.

Preparing the analyzer for shipment or storage

1. Shut off the process gas flow.
2. Allow all residual gas to dissipate from the lines.
3. Connect a purge supply, regulated to the specified sample supply pressure, to the sample supply port.
4. Confirm that any valves controlling the sample flow effluent to the low pressure flare or atmospheric vent are open.

5. Turn on the purge supply and purge the system to clear any residual process gases.
6. Turn off the purge supply.
7. Allow all residual gas to dissipate from the lines.
8. Close any valves controlling the sample flow effluent to the low pressure flare or atmospheric vent.
9. Disconnect power to the system.
10. Disconnect all tubing and signal connections.
11. Cap all inlets and outlets to prevent foreign material such as dust or water from entering the system.
12. Pack the equipment in the original packaging in which it was shipped, if available. If the original packaging material is no longer available, the equipment should be adequately secured (to prevent excessive shock or vibration).
13. If returning the analyzer to the factory, complete the Decontamination Form provided by Service and attach to the outside of the shipping package as instructed before shipping.

Storage

The packaged analyzer should be stored in a sheltered environment that is temperature controlled between -20 °C (-4 °F) and 50 °C (122 °F), and should not be exposed to rain, snow, caustic or corrosive environments. Humidity in the sheltered environment should be non-condensing.

Disclaimers

Endress+Hauser accepts no responsibility for consequential damages arising from the use of this equipment. Liability is limited to replacement and/or repair of defective components.

This manual contains information protected by copyright. No part of this guide may be photocopied or reproduced in any form without prior written consent from Endress+Hauser.

Warranty

For a period of 18 months from date of shipment or 12 months in operation, whichever comes first, Endress+Hauser warrants that all products sold by it shall be free from defects in material and workmanship under normal use and service when correctly installed and maintained. Endress+Hauser's sole liability and Customer's sole and exclusive remedy for a breach of warranty is limited to Endress+Hauser's repair or replacement (at Endress+Hauser's sole option) of the product or part thereof which is returned at Customer's expense to Endress+Hauser's plant. This warranty shall apply only if Customer notifies

Endress+Hauser in writing of the defective product promptly after the discovery of the defect and within the warranty period. Products may only be returned by Customer when accompanied by a return authorization reference number (SRO) issued by Endress+Hauser. Freight expenses for products returned by Customer will be prepaid by Customer. Endress+Hauser shall pay for shipment back to Customer for products repaired under warranty. For products returned for repair that are not covered under warranty, Endress+Hauser's standard repair charges shall be applicable in addition to all shipping expenses.

Appendix C: Analyzer Parts

This chapter provides lists and illustrations of all field replaceable parts used in the SS2100i-2 analyzer. Due to a policy of continuous improvement, parts and part numbers may change without notice.

Not all parts listed are included on every analyzer. When ordering, please specify the system serial number (S/N) to ensure that the correct parts are identified.

Table C-1 Electronics panel assembly parts

Figure Number	Reference Number	Part Number	Description
C-2	1	2100002097	One Phase Filter Model FN2415
C-1	2	EX4000000001	Power Supply, 100 to 240 VAC, 24 VDC / 1.3 A
C-2	3	4500002002	Relay, With Socket, C1D2, 6 A, DC12V, SPDT
C-2	4	4500002014	Thermostat, Manual Reset, 2455RM
C-2	5	8000002013	Assembly, Power Supply, Traco
C-1	6	2900000380	Assembly, PCB, Daughter, H ₂ S, ARM9
C-3	7	2900000450	Assembly, PCB, 4 to 20 mA, Dual Adjustable, Low Noise
C-1	8	4000002038	Temperature Controller, Watlow, EZ-ZONE RM
C-1	9	2800002063	Relay, 861 Solid State with Internal Heat Sink
C-3	10	2900000440	Assembly, Analog Input Board
C-1	11	2900000460	PCB, Assembly Temperature Control Hytek, 28 meter

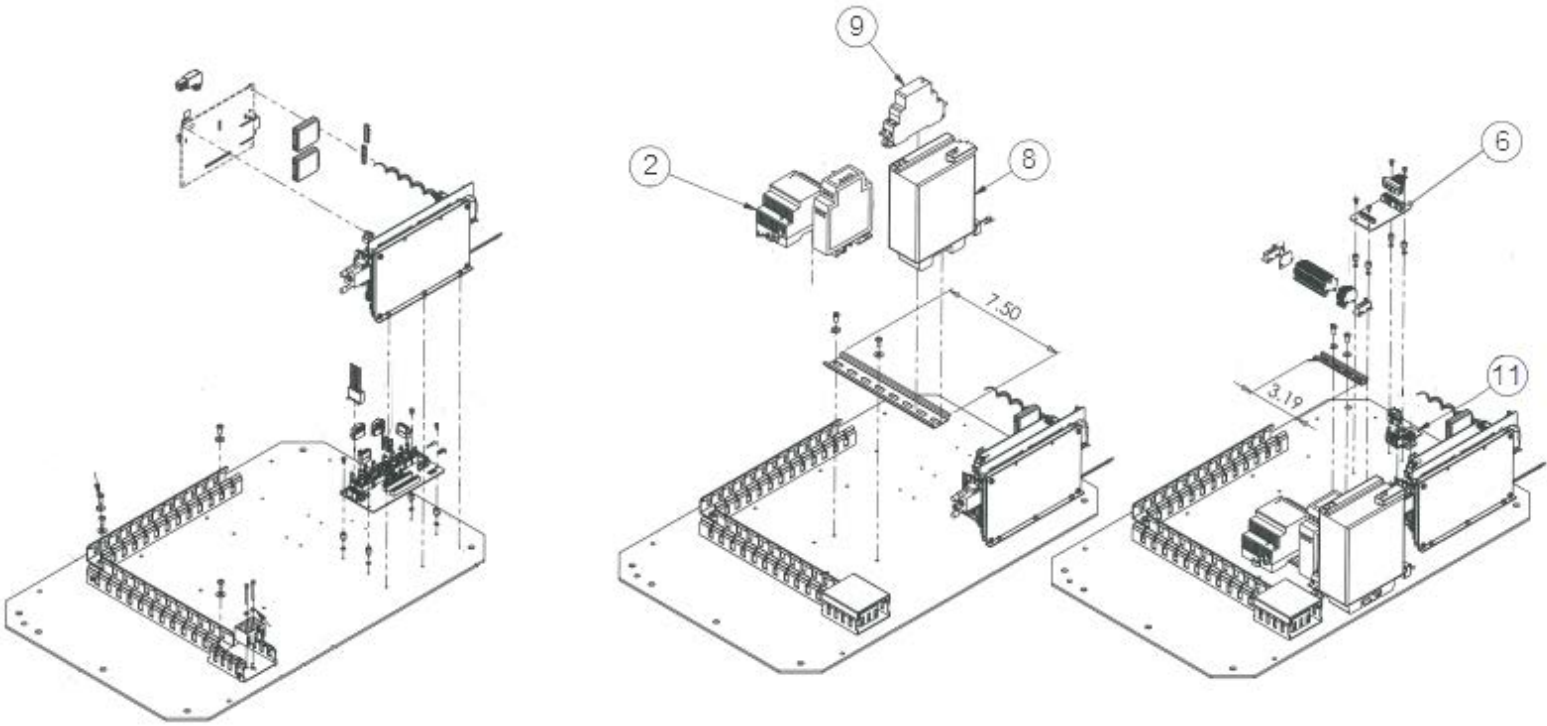


Figure C-1 Electronics panel assembly parts

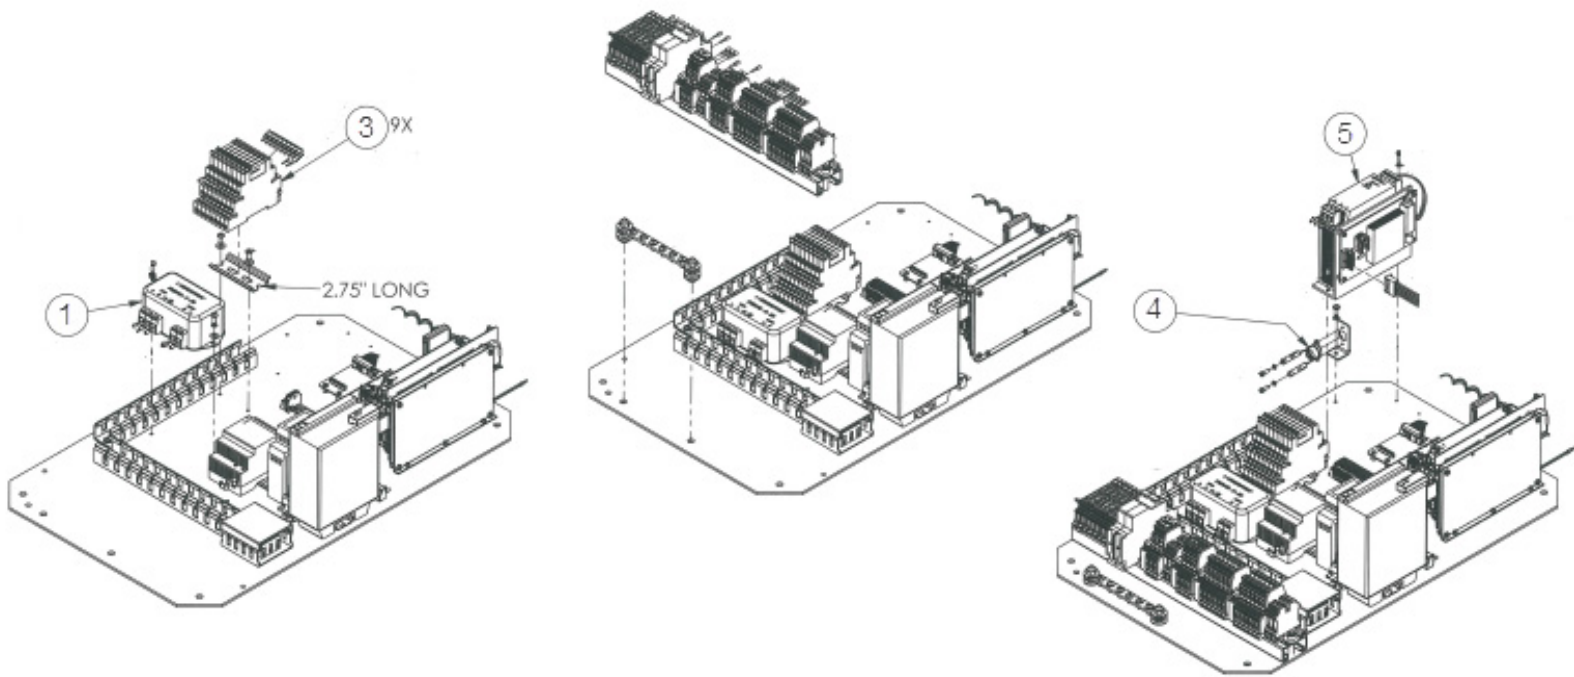


Figure C-2 Electronics panel assembly parts (Continued)

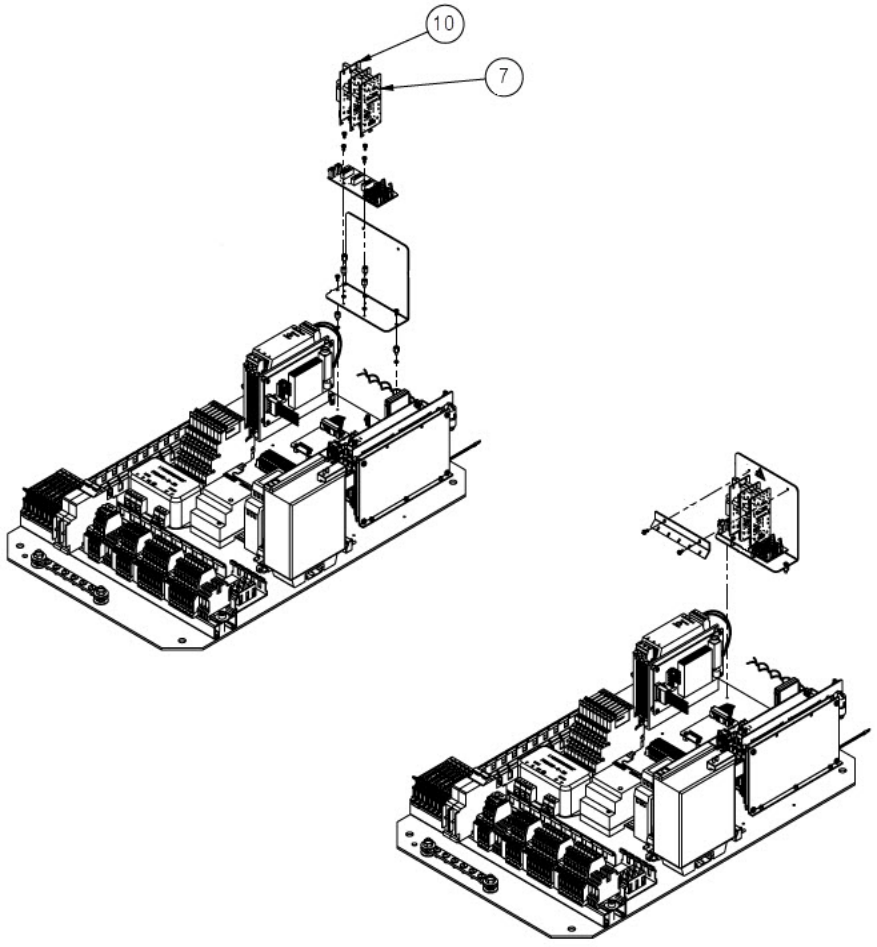
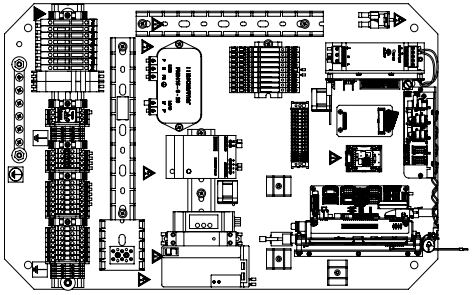


Figure C-3 Electronics panel assembly parts (Continued)

Table C-2 *Field interface terminal block assembly parts*

Figure Number	Reference Number	Part Number	Description
C-4	1	4500002015	Circuit Breaker, 9926 Series
C-4	2	2100002086	Terminal Block Fuse, UK 5-HESILA 250, Un-500V, In-6.3A
C-4	3	4500002010 ¹	Fuse, Miniature, 5 x 20 mm, 0.5 A
C-4	4	4500002011 ¹	Fuse, Miniature, 5 x 20 mm, 0.1 A
C-4	5	4500002012 ¹	Fuse, Miniature, 5 x 20 mm, 1 A
C-4	6	4500002013 ¹	Fuse, Miniature, 5 x 20 mm, 1.2 A

1. See Table 1-1 on page 1-15 or Table 1-2 on page 1-16 for additional fuse specifications.

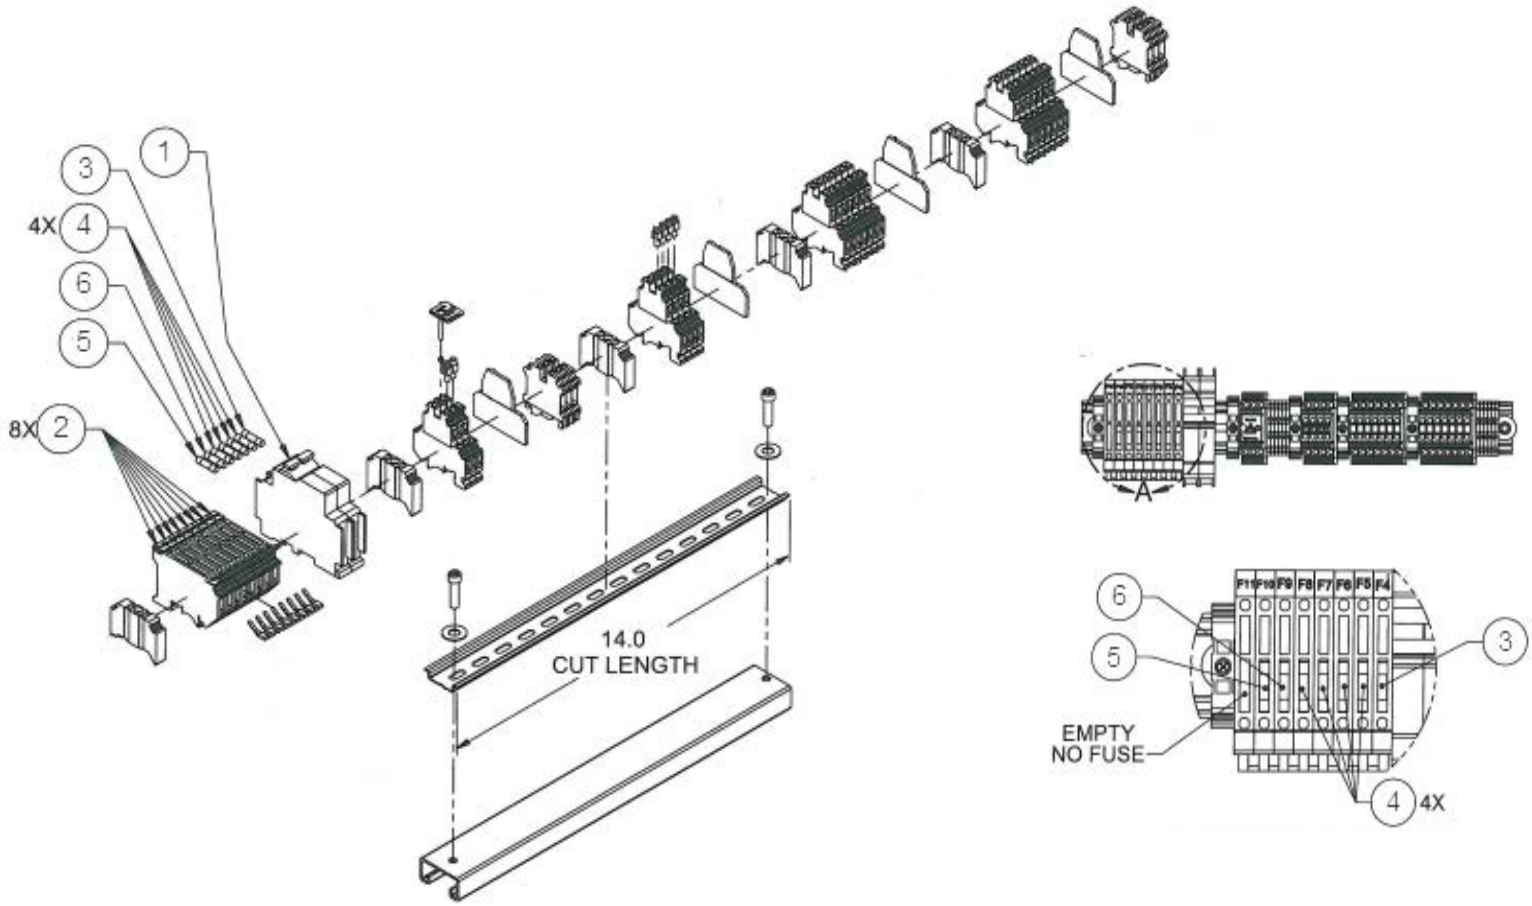


Figure C-4 Field interface terminal block assembly

Table C-3 Parts for 8/28 m sample cell panel assembly

Figure Number	Reference Number	Part Number	Description
C-5	1	EX5300000001	Heater, 230VAC, 200W, EExd IIC T3
		EX5300000002	Heater, 120VAC, 200W, EExd IIC T3
C-6	2	2400002085	DC Series Tube axial Cooling Fan, Model:D36T10
C-6	3	5500002017	Assembly, Thermistor Probe, ATEX
C-8	4	5500002041	Pressure Sensor, 30 PSIA, 5 V, 1/8 in. MNPT DIN4365, NACE ¹

1. Contact Endress+Hauser Service department before attempting replacement. Replacing this component without Service support could cause damage to other components. For Service, refer to our website for the list of local sales channels in your area (www.endress.com).

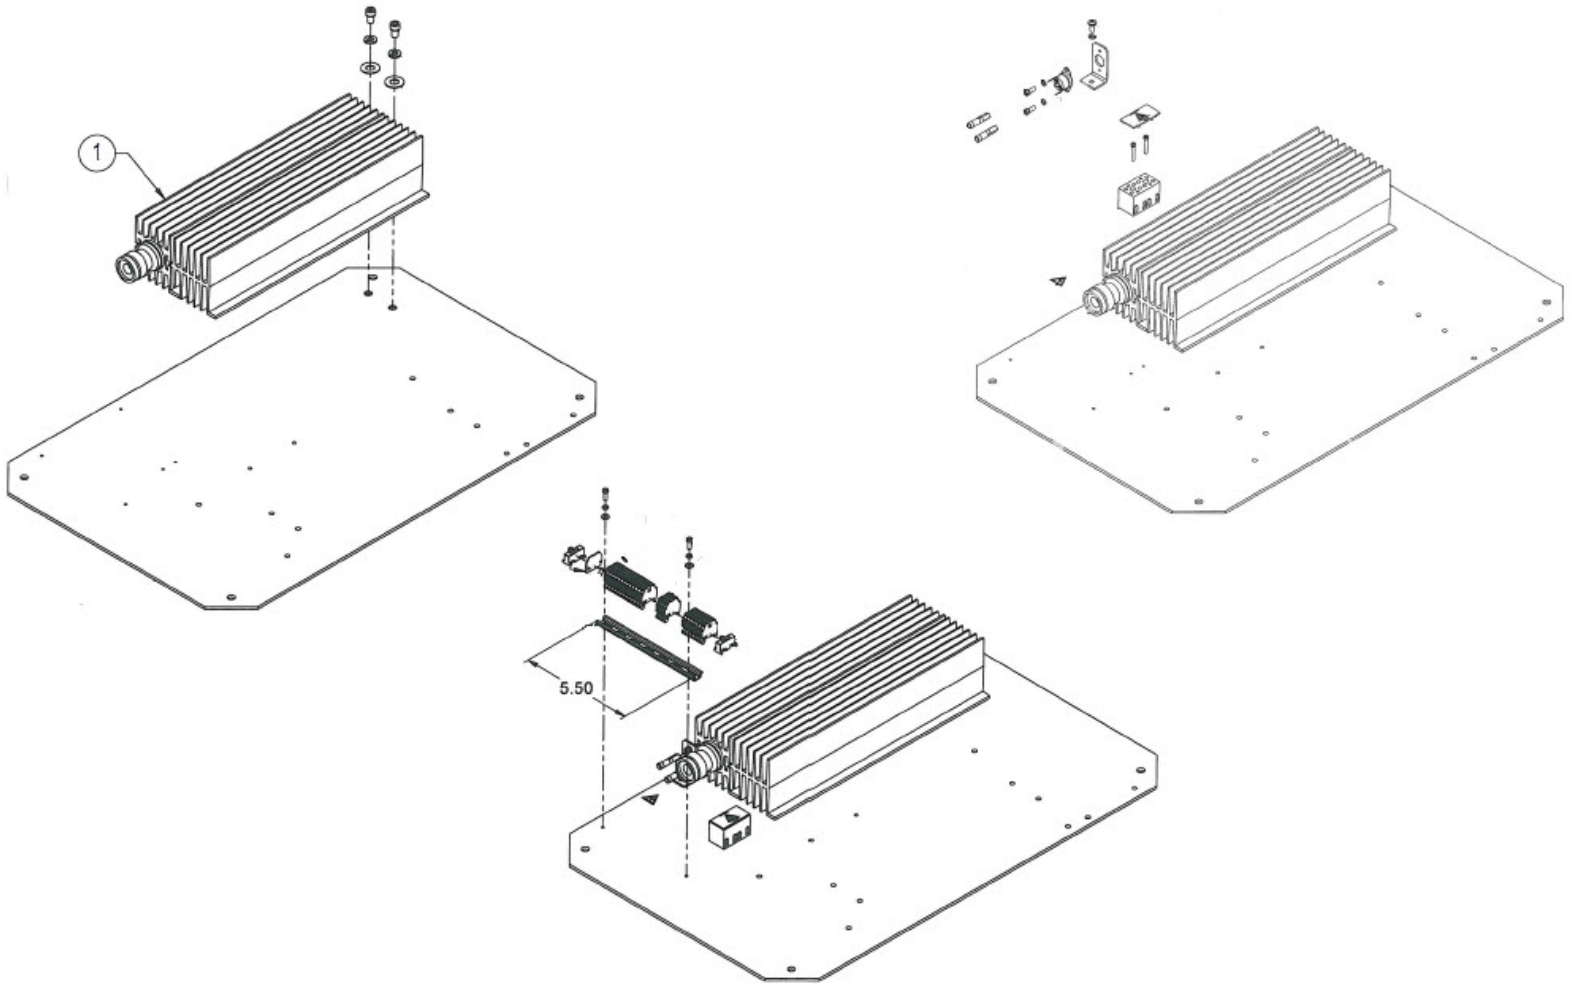


Figure C-5 8/28 m sample cell panel assembly parts

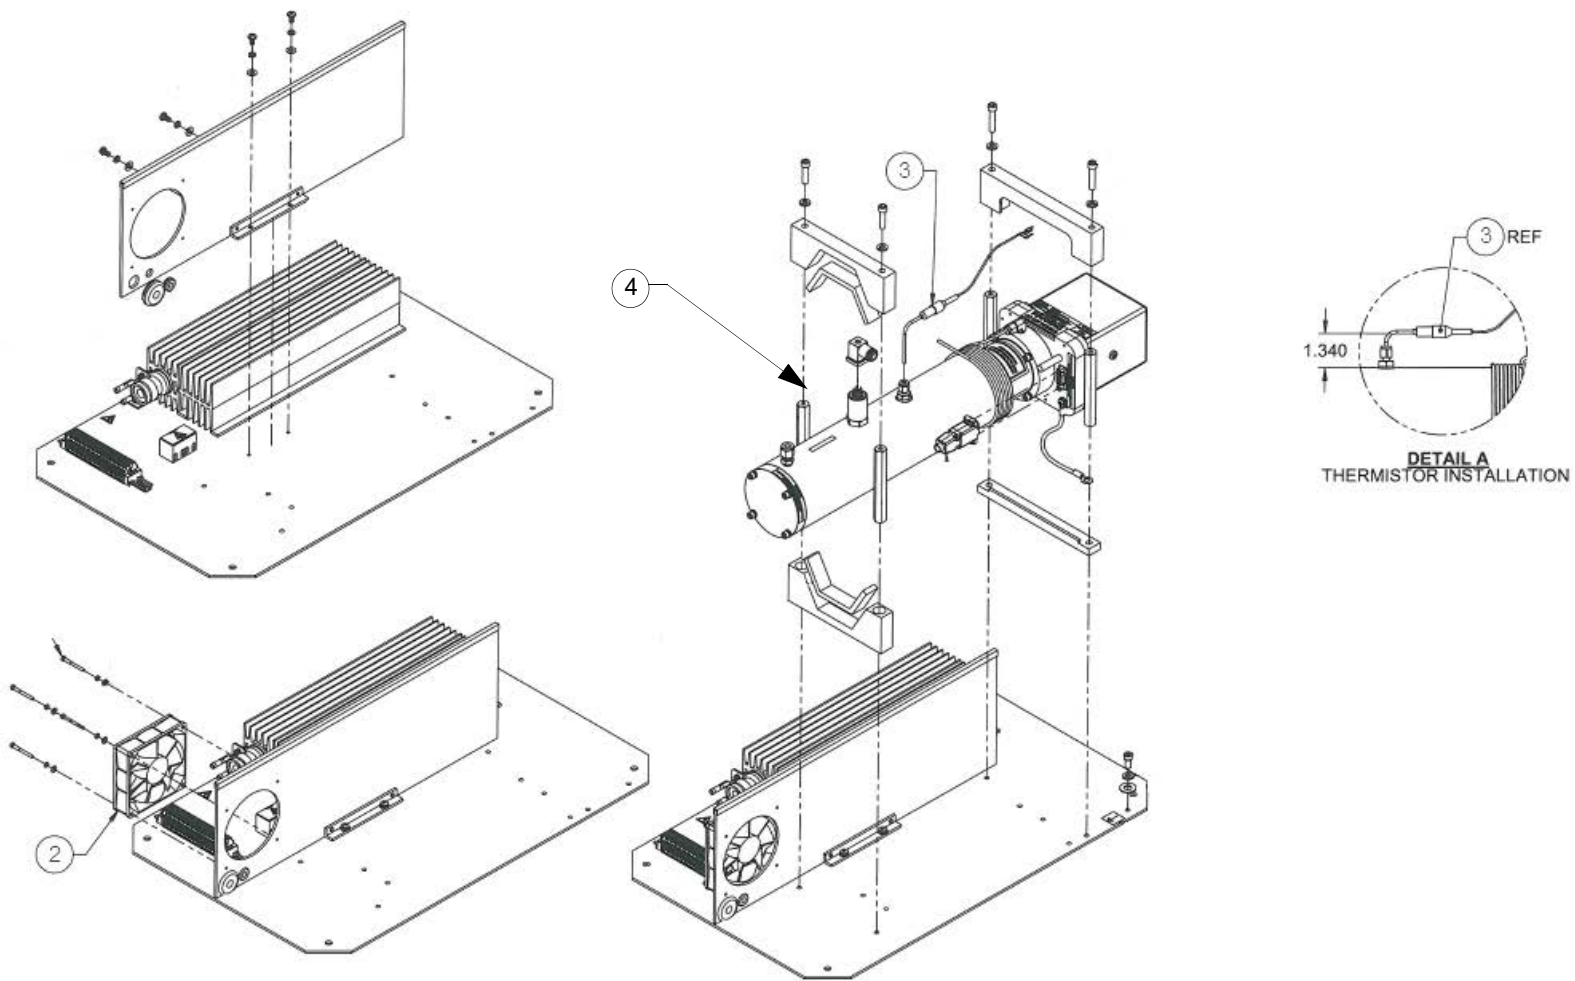


Figure C-6 8/28 m sample cell panel assembly parts (Continued)

Table C-4 Parts for 0.8 m sample cell panel assembly

Figure Number	Reference Number	Part Number	Description
C-7	1	EX5300000001	Heater, 230 VAC, 200W, EExd IIC T3
		EX5300000002	Heater, 120VAC, 200W, EExd IIC T3
C-8	2	2400002085	DC Series Tube axial Cooling Fan, Model:D36T10
C-8	3	5500002041	Pressure Sensor, 30 PSIA, 5V, 1/8 in. MNPT DIN4365, NACE ¹
C-8	4	5500002023	Assembly, Thermistor Probe, ATEX
C-8	5	0900002146	Stainless Steel Mirror

1. Contact Endress+Hauser Service department before attempting replacement. Replacing this component without Service support could cause damage to other components. For Service, refer to our website for the list of local sales channels in your area (www.endress.com).

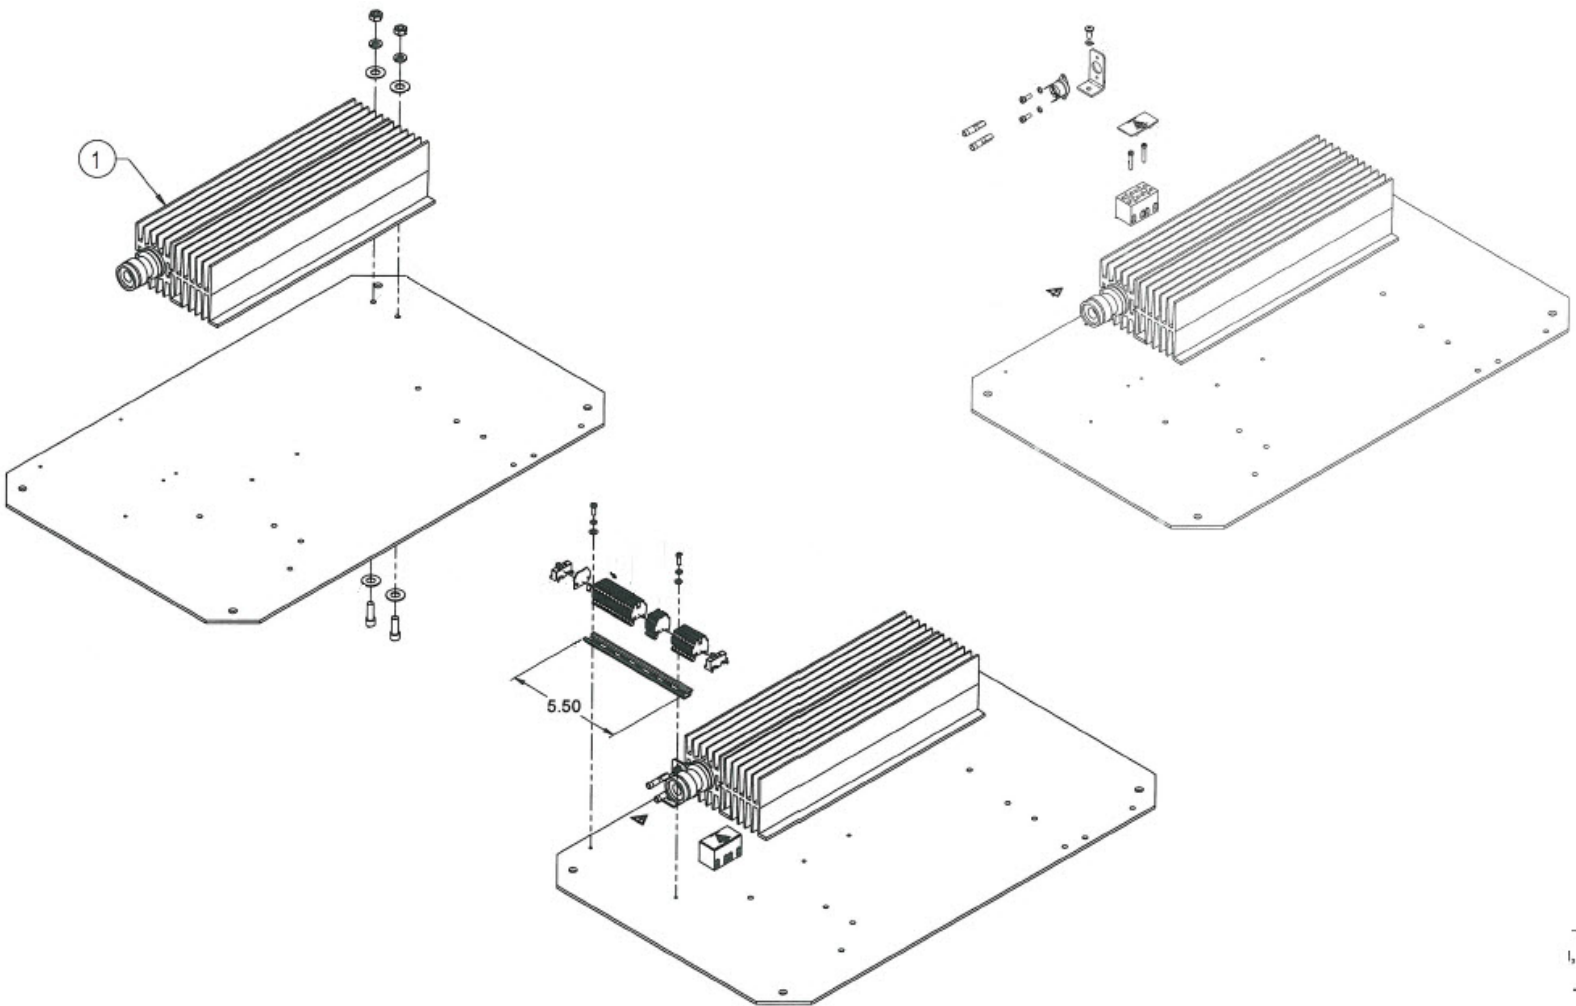


Figure C-7 0.8 m sample cell panel assembly parts

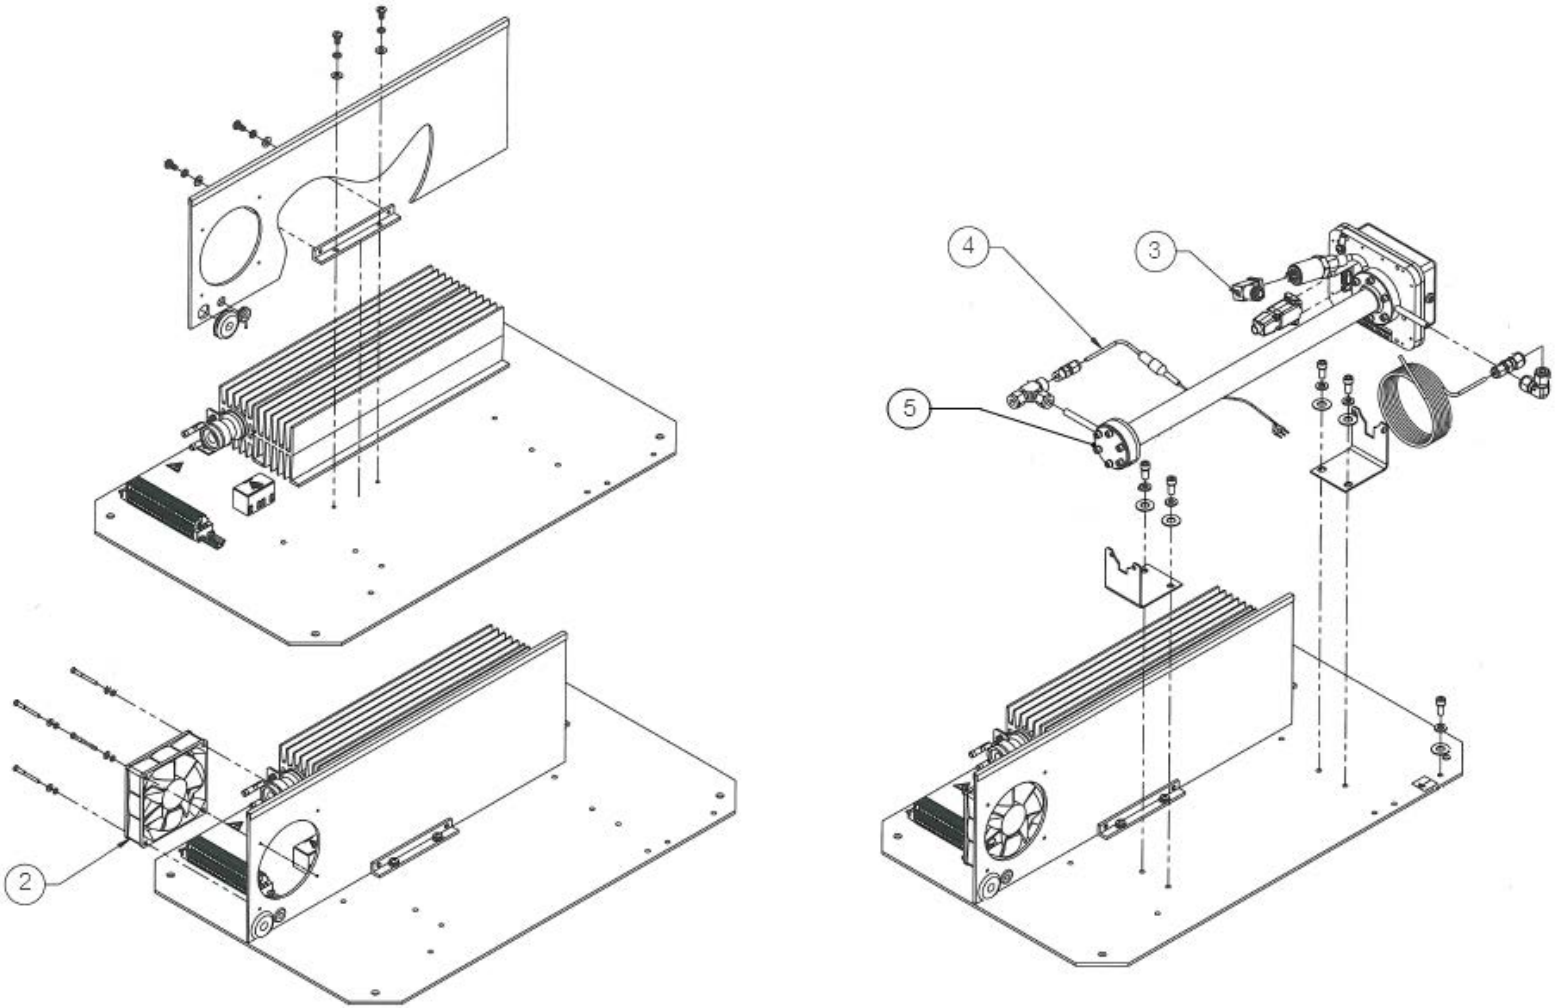


Figure C-8 0.8 m sample cell panel assembly parts (Continued)

Table C-5 Parts for 0.1 m sample cell panel assembly

Figure Number	Reference Number	Part Number	Description
C-9	1	EX5300000001	Heater, 230 VAC, 200 W, EExd IIC T3
		EX5300000002	Heater, 120 VAC, 200 W, EExd IIC T3
C-10	2	2400002085	DC Series Tube axial Cooling Fan, Model:D36T10
C-10	3	5500002041	Pressure Sensor, 30 PSIA, 5 V, 1/8 in. MNPT DIN4365, NACE ¹
C-10	4	5500002023	Assembly, Thermistor Probe, ATEX
C-10	5	0900002146	Stainless Steel Mirror

1. Contact Endress+Hauser Service department before attempting replacement. Replacing this component without Service support could cause damage to other components. For Service, refer to our website for the list of local sales channels in your area (www.endress.com).

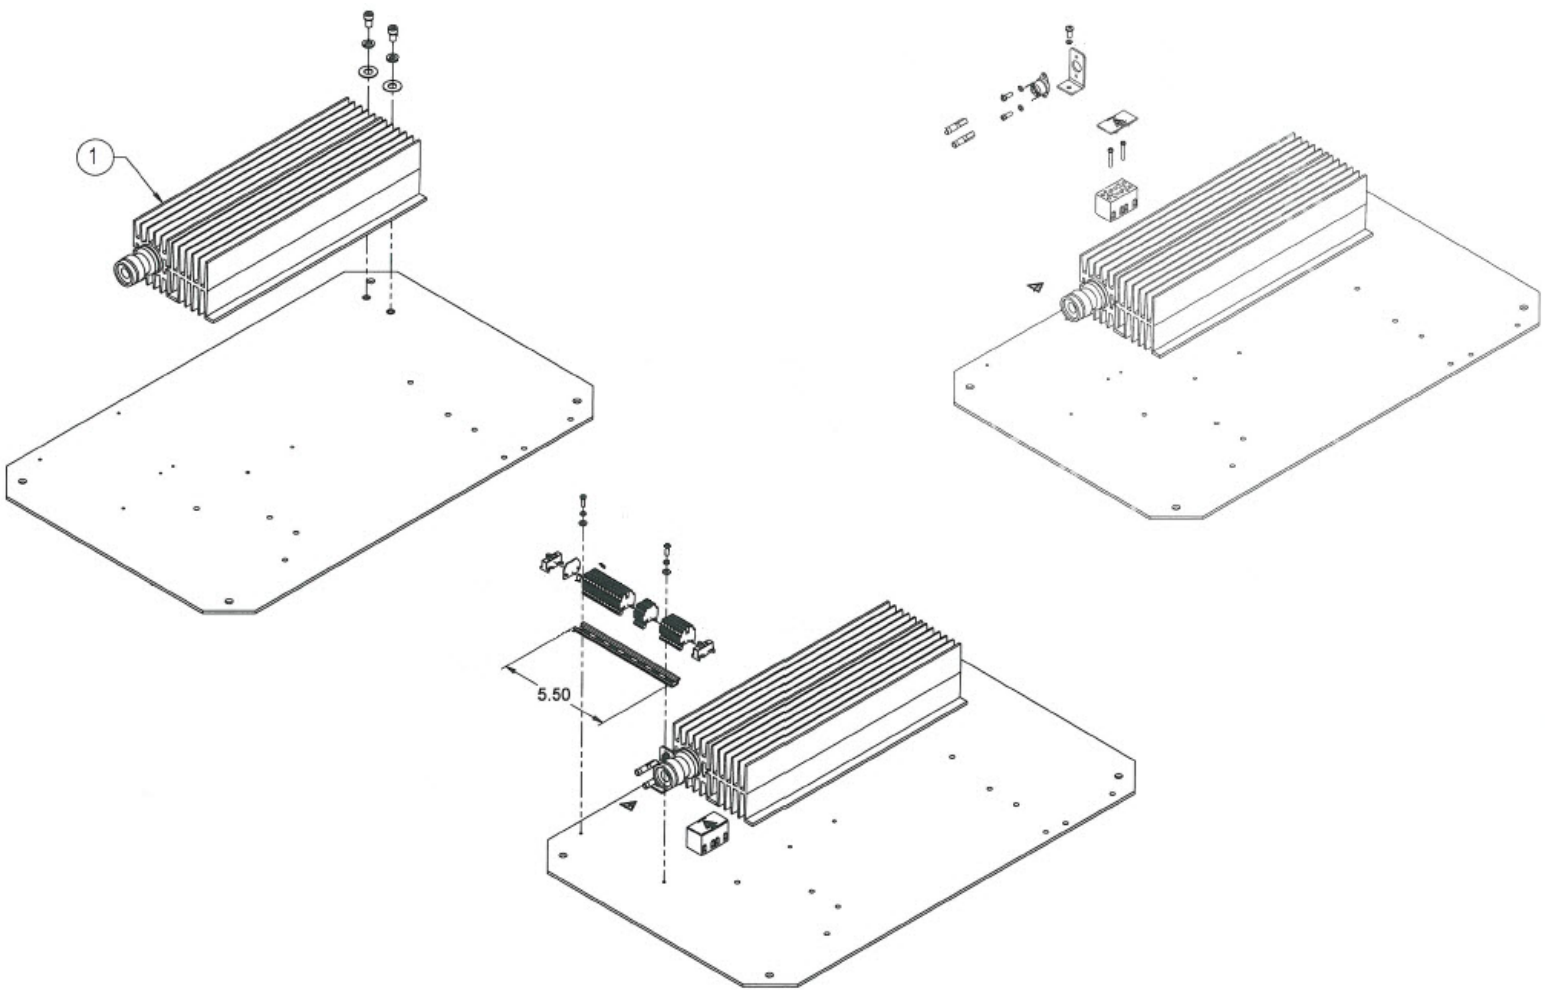


Figure C-9 0.1 m sample cell panel assembly parts

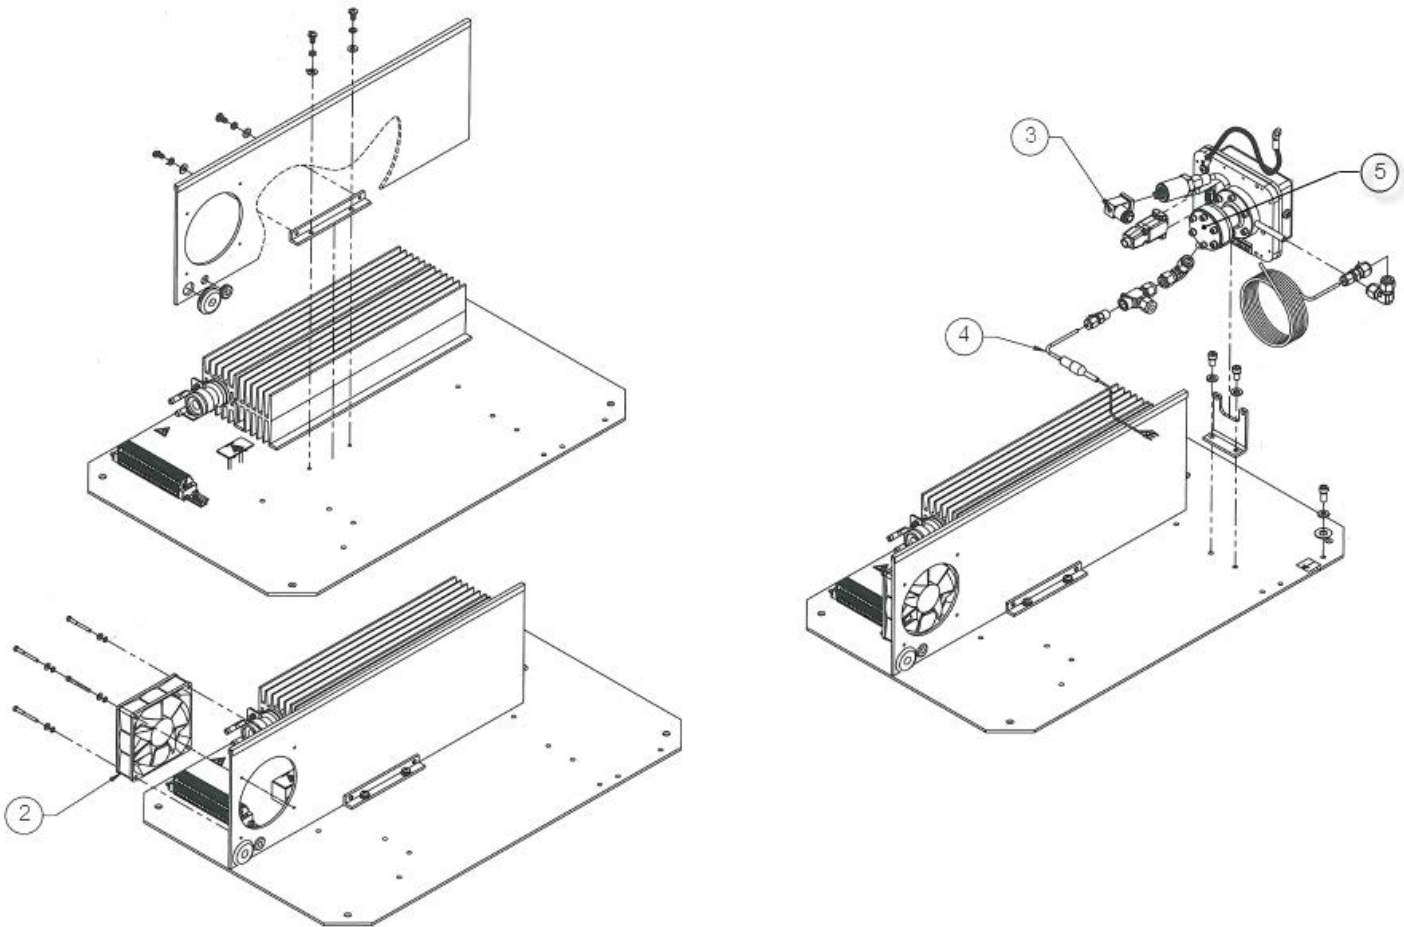


Figure C-10 0.1 m sample cell panel assembly parts (Continued)

Table C-6 Parts for electronics enclosure assembly

Figure Number	Reference Number	Part Number	Description
C-11	1	2400002157	Keypad, Touch Sensitive, 16 Keys
C-11	2	2400002161	Display, LCD, 20X4, Backlit, 5 V, Serial

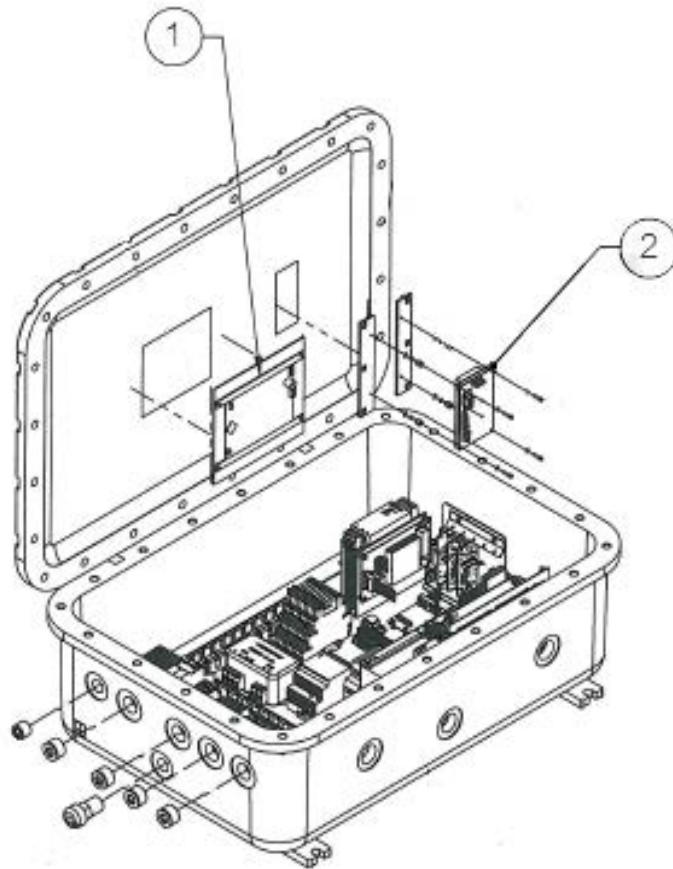


Figure C-11 Analyzer electronics enclosure assembly

Table C-7 Service parts

Part Number	Description
5500002022	Transition Plate Thermistor
Cables	
6000002148	Assembly, Cable, Pressure Sensor, GP50, Cell Enclosure (all cell sizes)
6000002201	Cable, Pressure Sensor, GP50, 35 in.
6000002139	Assembly, Cable, Pressure Sensor, GP50, Electrical Enclosure (to Backplane Connector)
6000002146	Assembly, Cable Optical Head, EExd, Electrical Enclosure
6000002021	Assembly, Cable, Signal, Optical Head
6000002138	Assembly, Cable, Thermistor Cell, Electrical Enclosure
6000002203	Assembly, Cable Thermistor Cell, Backplane
6000002152	Assembly, Cable, Relay Interface, ARM9 (EExd ENCL)
6000002193	Assembly, Ethernet Cable, CAT5e
6000002189	Cable, Harness, Signal Output RS-232/4-20 mA
6000002261	Cable, Harness, Signal Output RS-232/4-20 mA 25 in.
6000002192	Assembly, Cable, 4-20 mA Input
6000002191	Assembly, Cable, 4-20 mA Output
6000002204	Assembly, Cable, AI Jumper, J8 to J4
6000002158	Assembly, Cable, RS-232, M-M, Display, Data (EExd)
6000002159	Assembly, Cable, Power, Display (EExd)
0190217204	Cable, Power Supply Output, 14 in.
0190217208	Cable, TE Cooler
0190217205	Harness, Ribbon, 10 Conductor, 9 in.
Scrubber/Indicator (Differential Systems Only)	
8000002209	Kit, H ₂ S Scrubber/Indicator, 3 in. Diameter
8000002207	Kit, H ₂ S Scrubber/Indicator, 2 in. Diameter
8000002205	Kit, NH ₃ Scrubber/Indicator, 3 in. Diameter
8000002224	Kit, NH ₃ Scrubber/Indicator, 2 in. Diameter
8000002205	Kit, HCl Scrubber/Indicator, 3 in. Diameter
8000002224	Kit, HCl Scrubber/Indicator, 2 in. Diameter
6101811014	Dryer, NuPure

Table C-7 Service parts (Continued)

Part Number	Description
Hardware/Kits	
0219900006	Kit, Spares (O-rings, screws), Viton, 8/28 m Cell
0219900005	Kit, Spares (O-rings, screws), Viton, 0.8 m Cell
1300002427	Washer, Sealing, SS, M10
1300002425	Screw, Socket Head Cap, 304SS, M10x35
1300002426	Screw, Socket Head Cap, 304SS, M10x30
1100002210	Kit, SS2100i-2, M10x35 Bolts and M10 Washer
0219900007	Kit, Cleaning Tools, Optical Cell (USA/Canada) ¹
0219900017	Kit, Cleaning Tools, Optical Cell (International) ¹
1100002156	Tooling Kit (Installation/Maintenance)
General	
BA02197C	SS2100i-2 TDLAS Gas Analyzer Operating Instruction, additional copies
GP01177C	Description of Device Parameters FS 5.16, additional copies
XA02694C	SS2100i-2 TDLAS Gas Analyzer Safety Instruction, additional copies
GP01180C	Description of Device Parameters NS 5.14, additional copies

1. Contact Endress+Hauser Service department before attempting replacement. Replacing this component without Service support could cause damage to other components. For Service, refer to our website for the list of local sales channels in your area (www.endress.com).

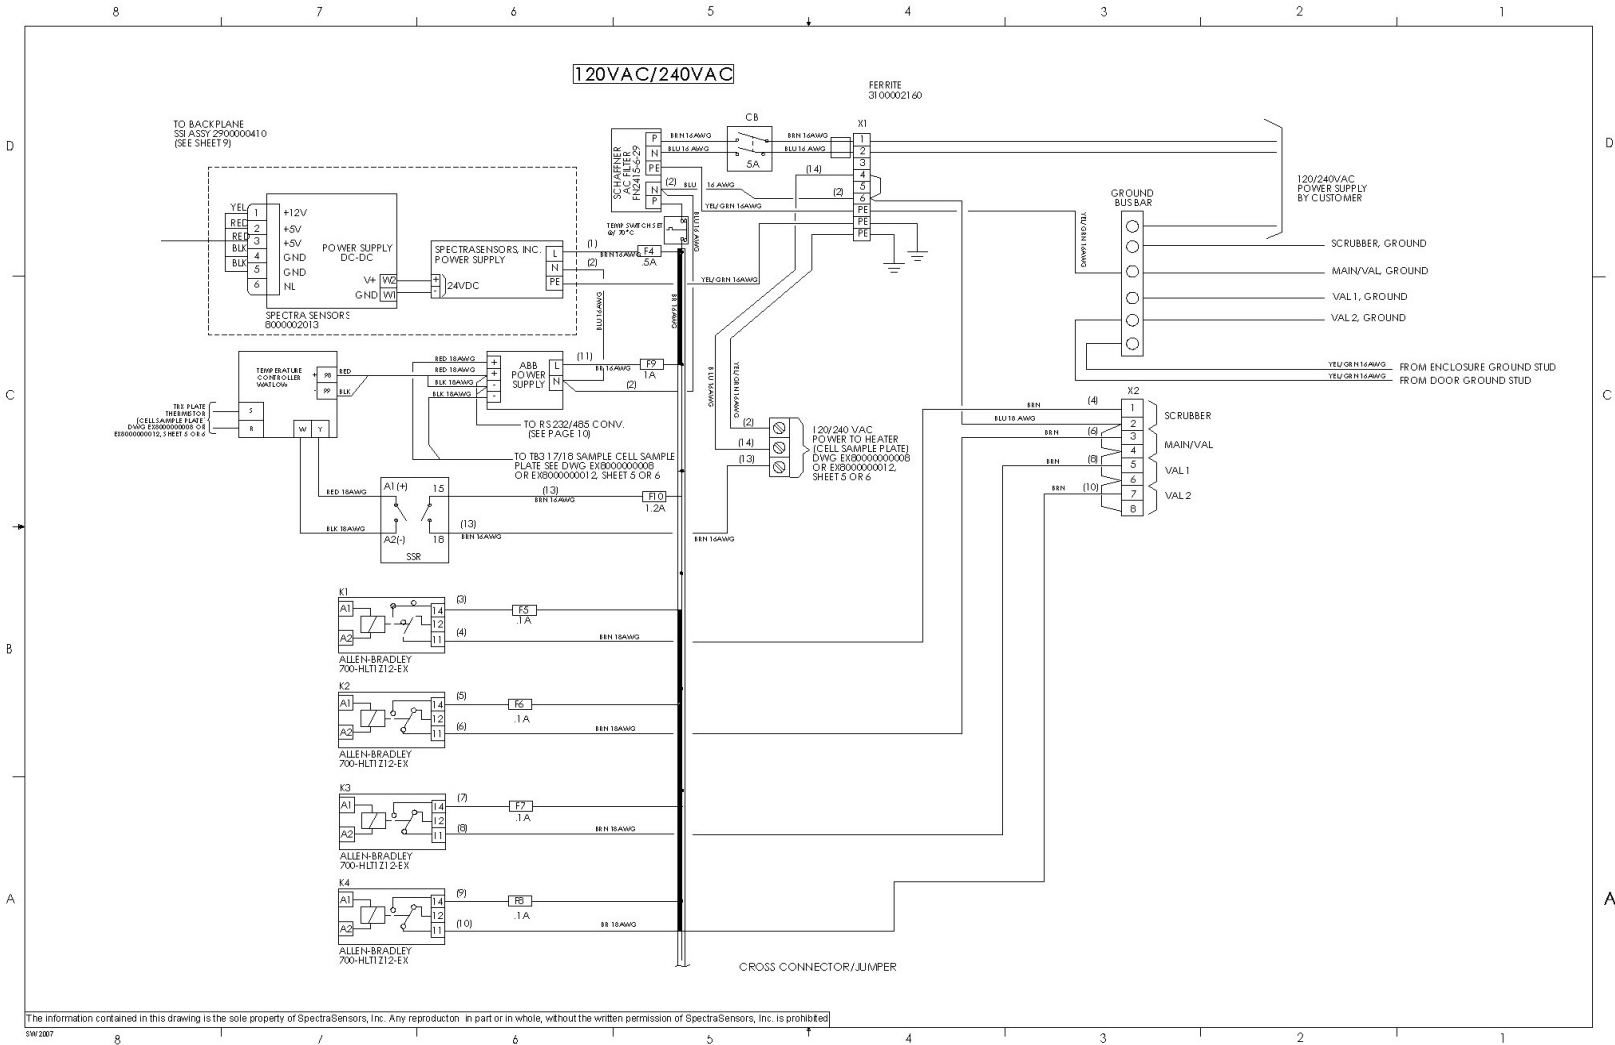


Figure D-1 Wiring schematic of SS2100i-2 electronics power systems



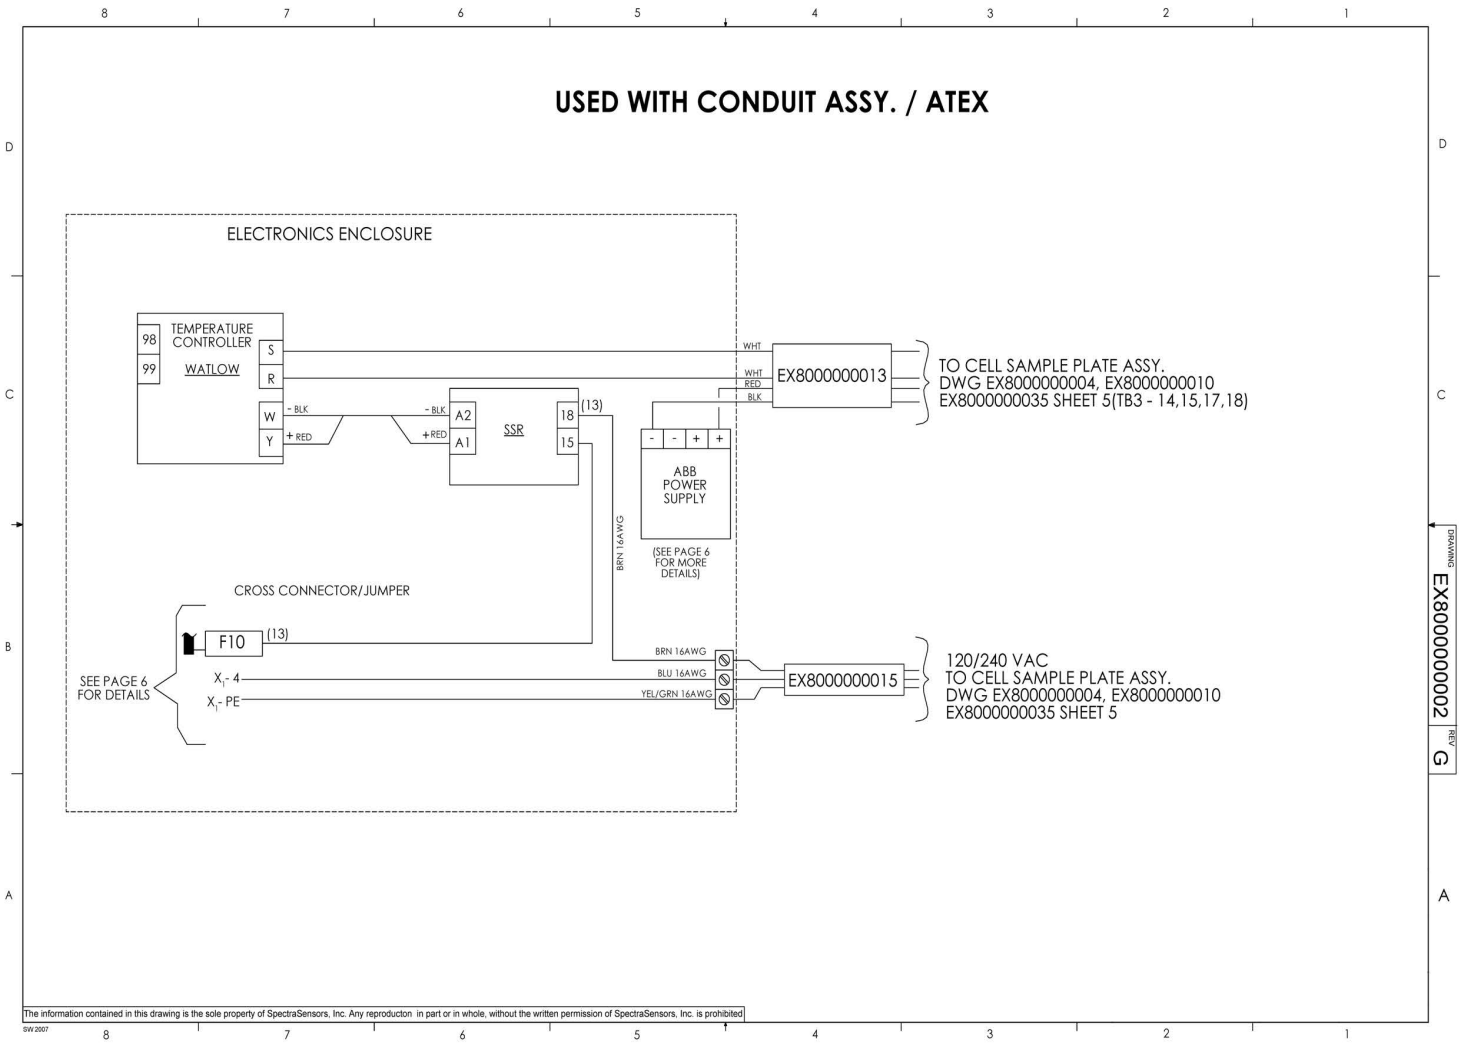


Figure D-2 Wiring schematic of conduit-coupled SS2100i-2 power system

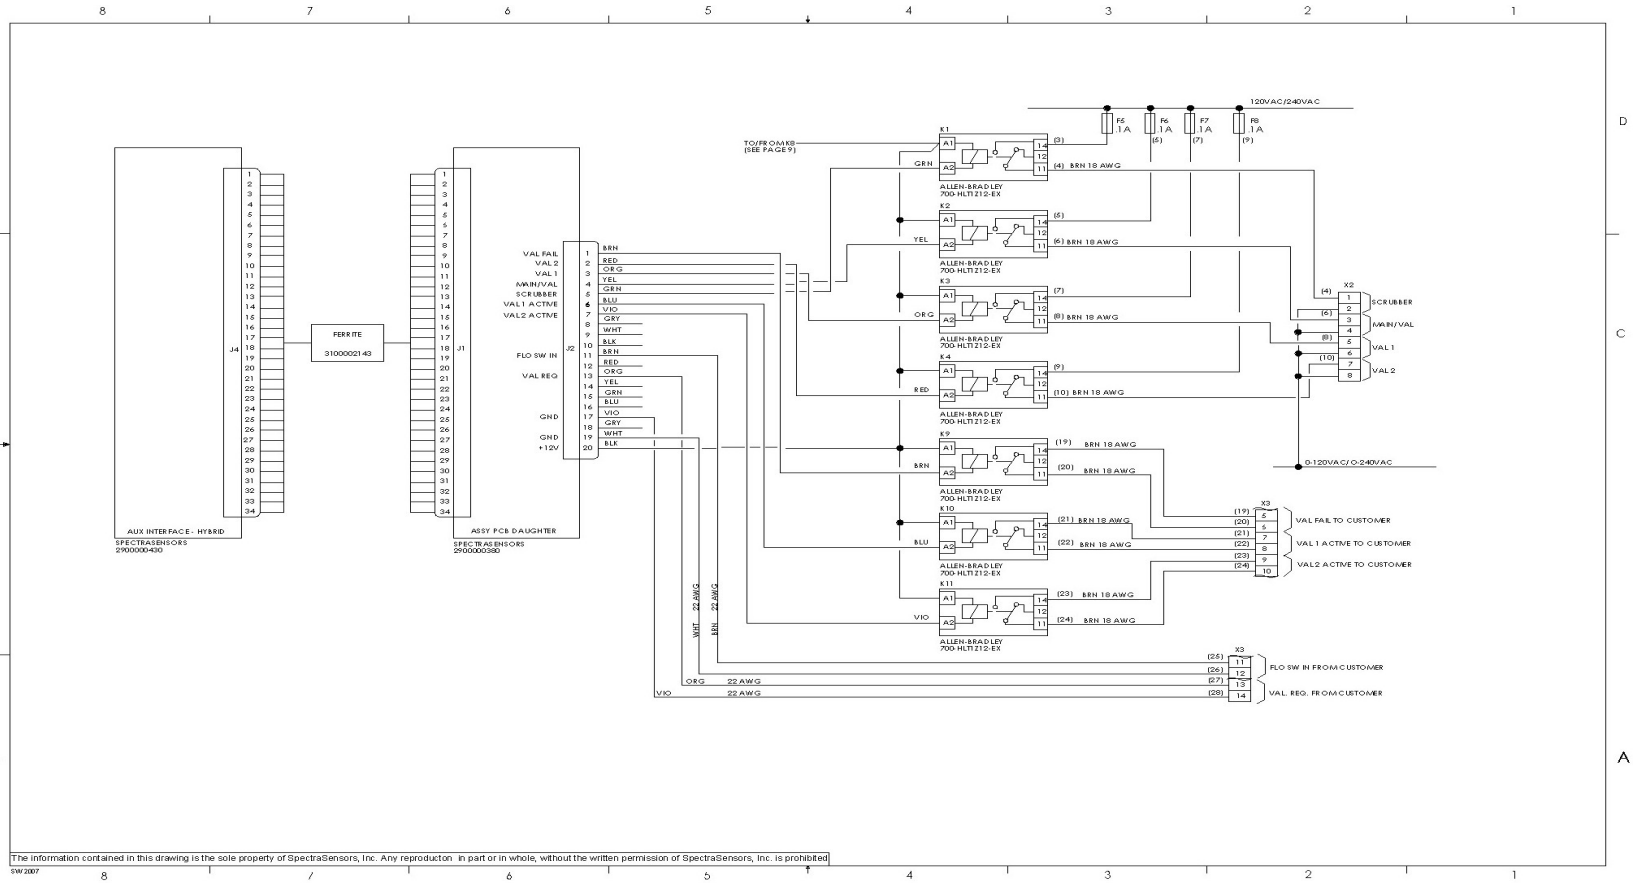

The information contained in this drawing is the sole property of SpectraSensors, Inc. Any reproduction in part or in whole, without the written permission of SpectraSensors, Inc. is prohibited.
SW 2007

Figure D-3 Wiring schematic of SS2100i-2 digital I/O

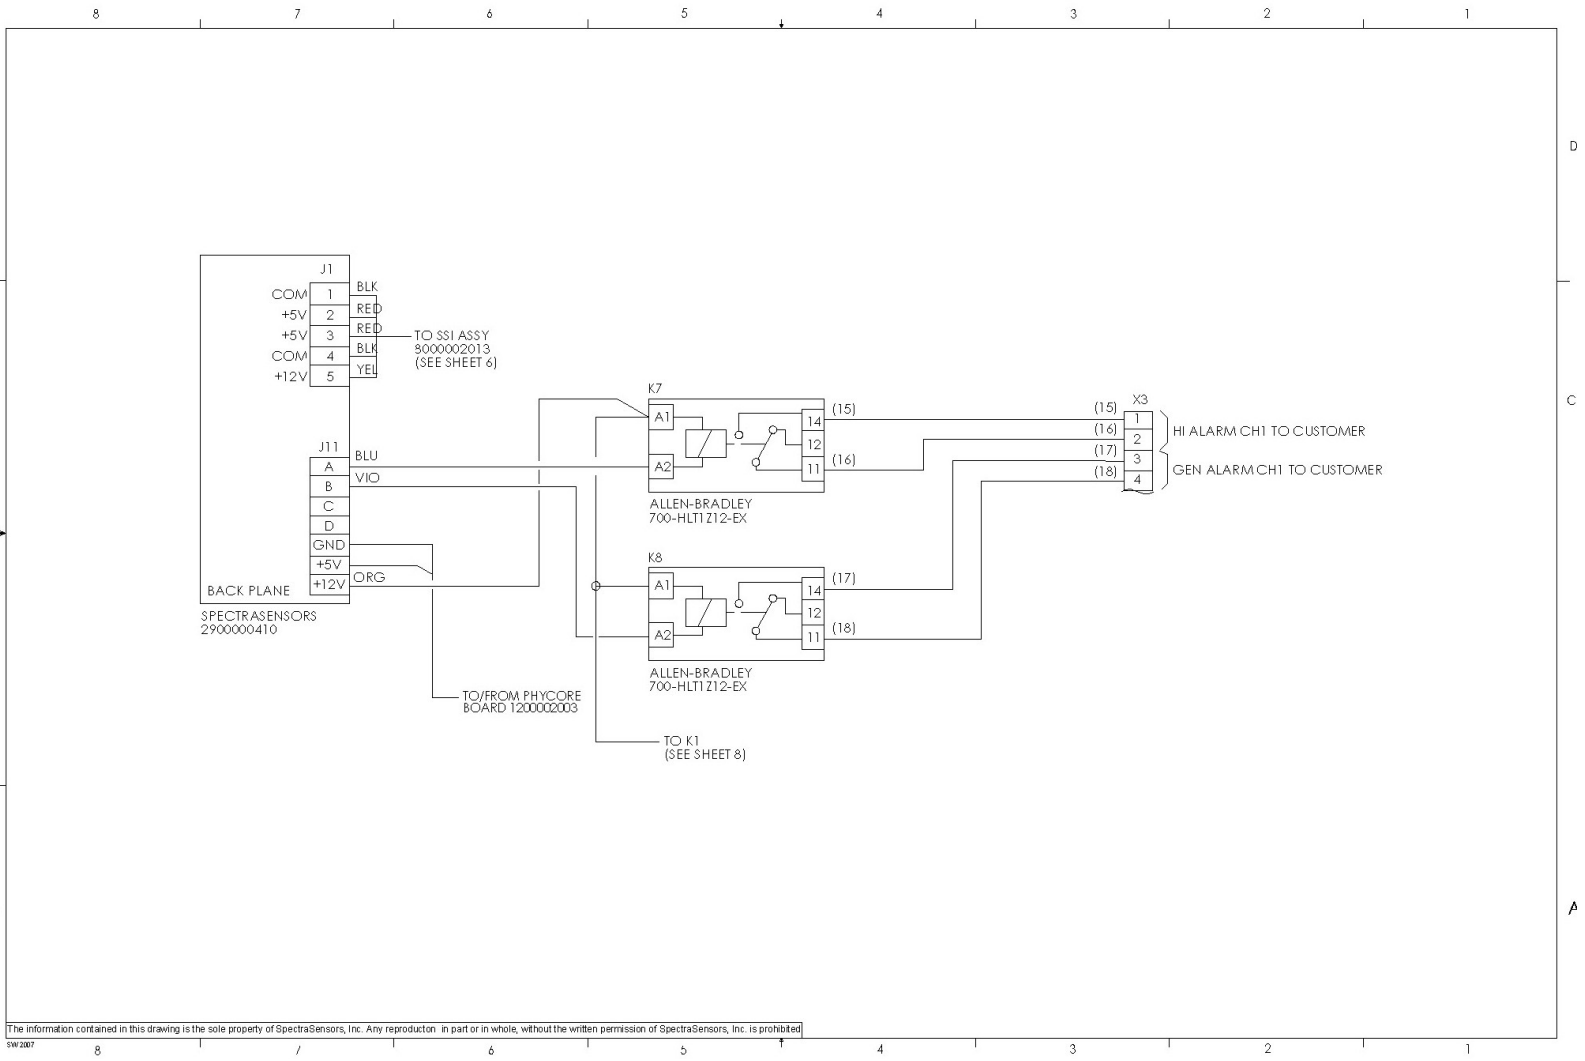

The information contained in this drawing is the sole property of SpectraSensors, Inc. Any reproduction in part or in whole, without the written permission of SpectraSensors, Inc. is prohibited.

Figure D-4 Wiring schematic of SS2100i-2 alarms


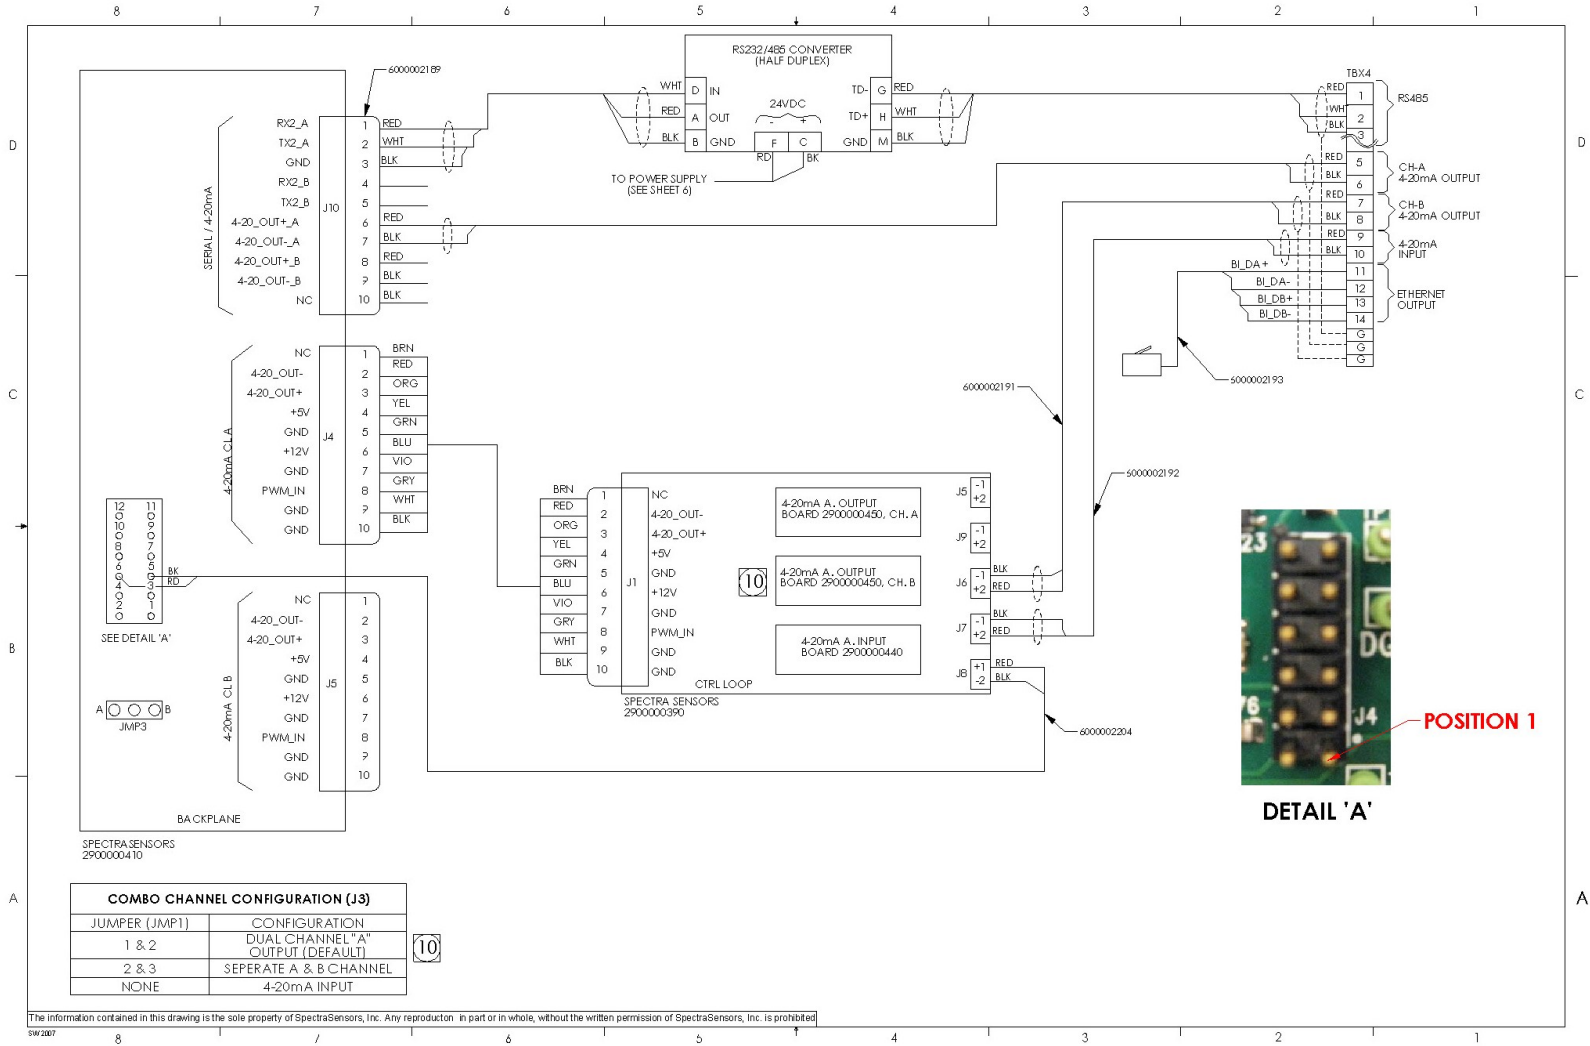


Figure D-5 Wiring schematic of SS2100i-2 serial and Ethernet signals

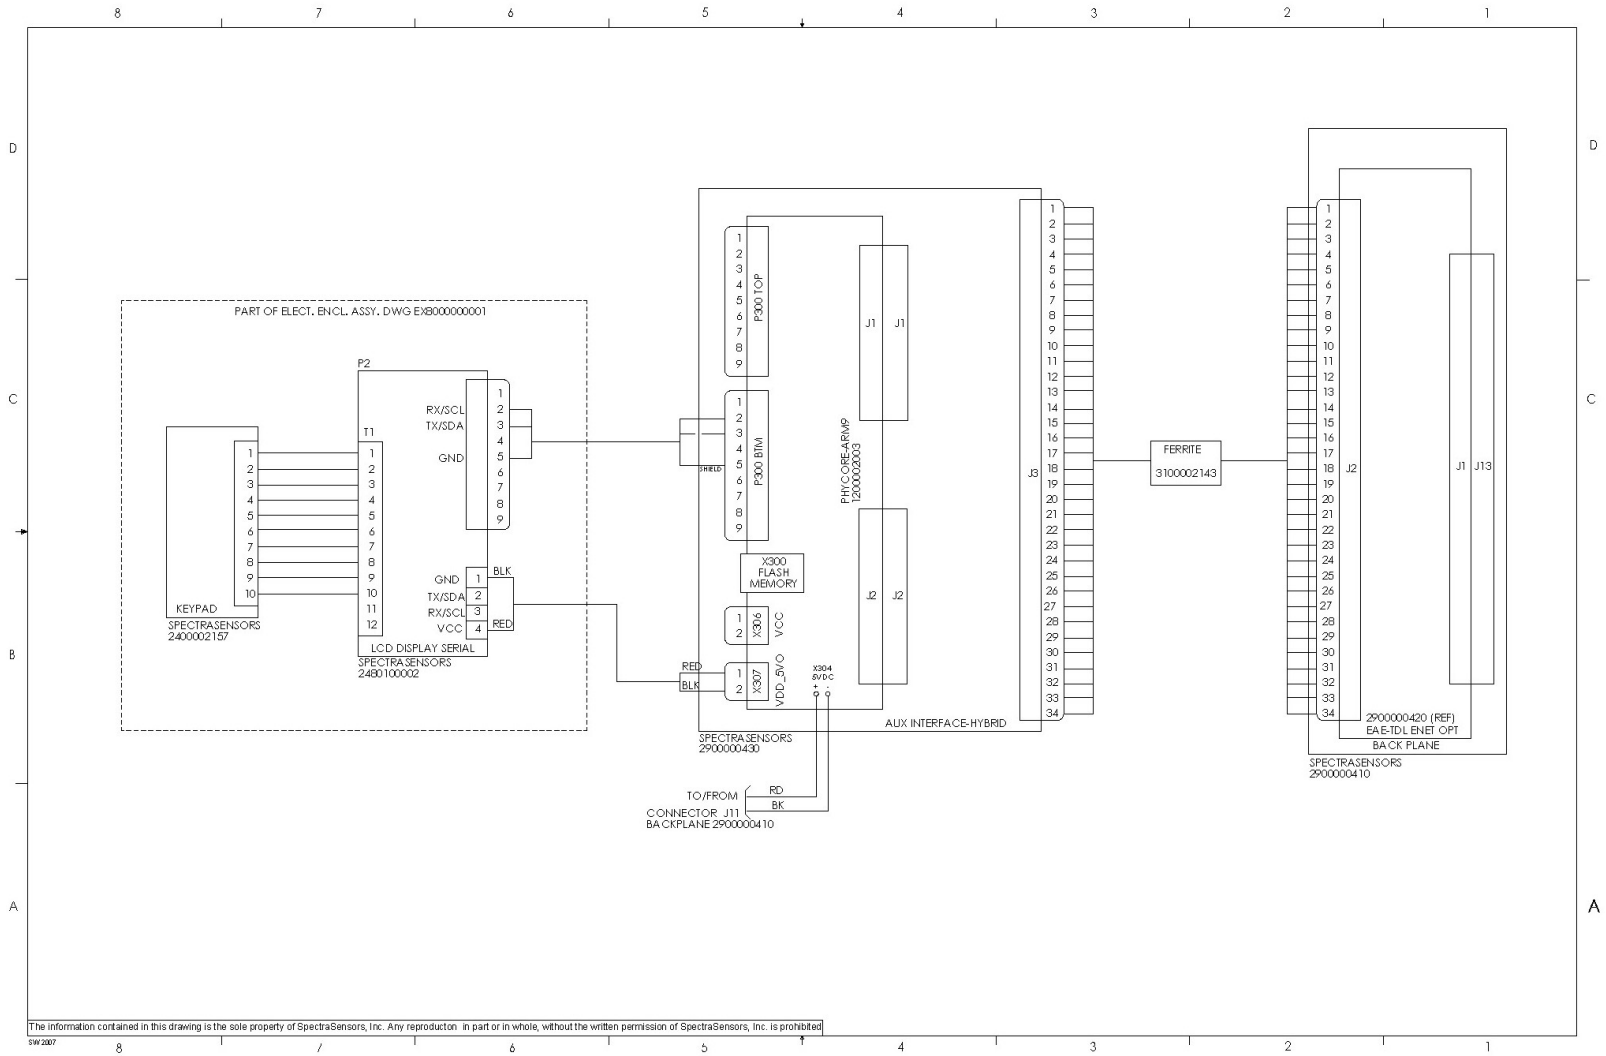

The information contained in this drawing is the sole property of SpectraSensors, Inc. Any reproduction in part or in whole, without the written permission of SpectraSensors, Inc. is prohibited.
 SW 2207

Figure D-6 Wiring schematic of SS2100i-2 inter-card connections

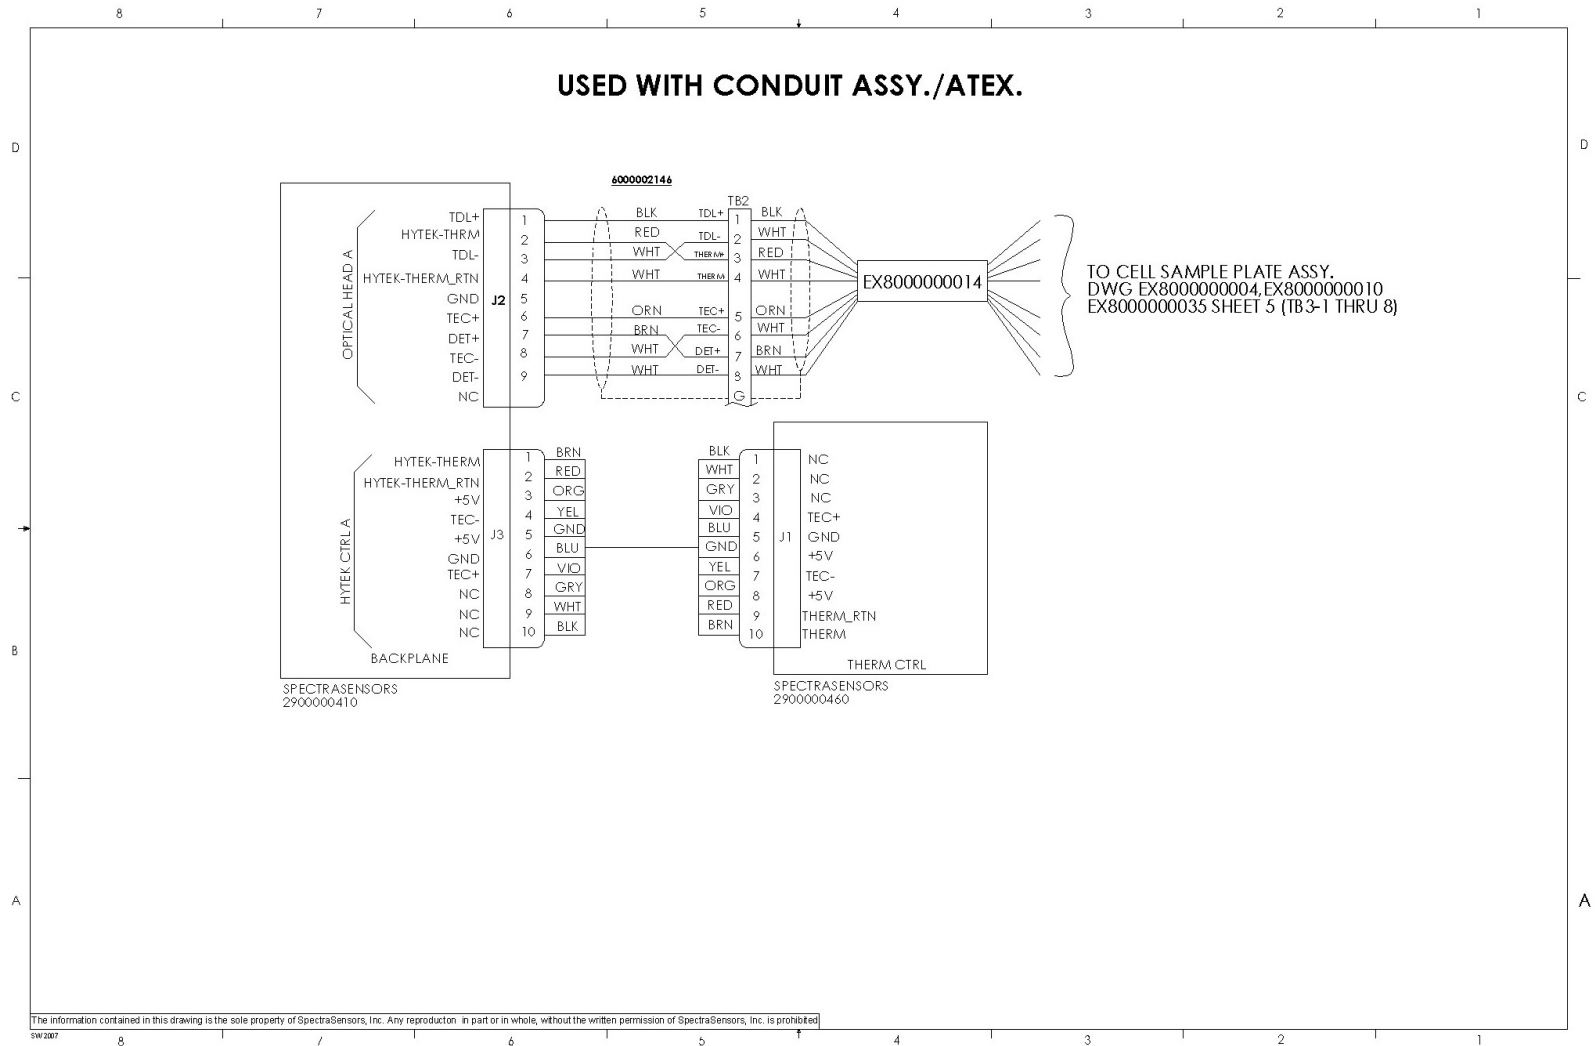


Figure D-7 Wiring schematic of conduit-coupled SS2100i-2 optical head connections

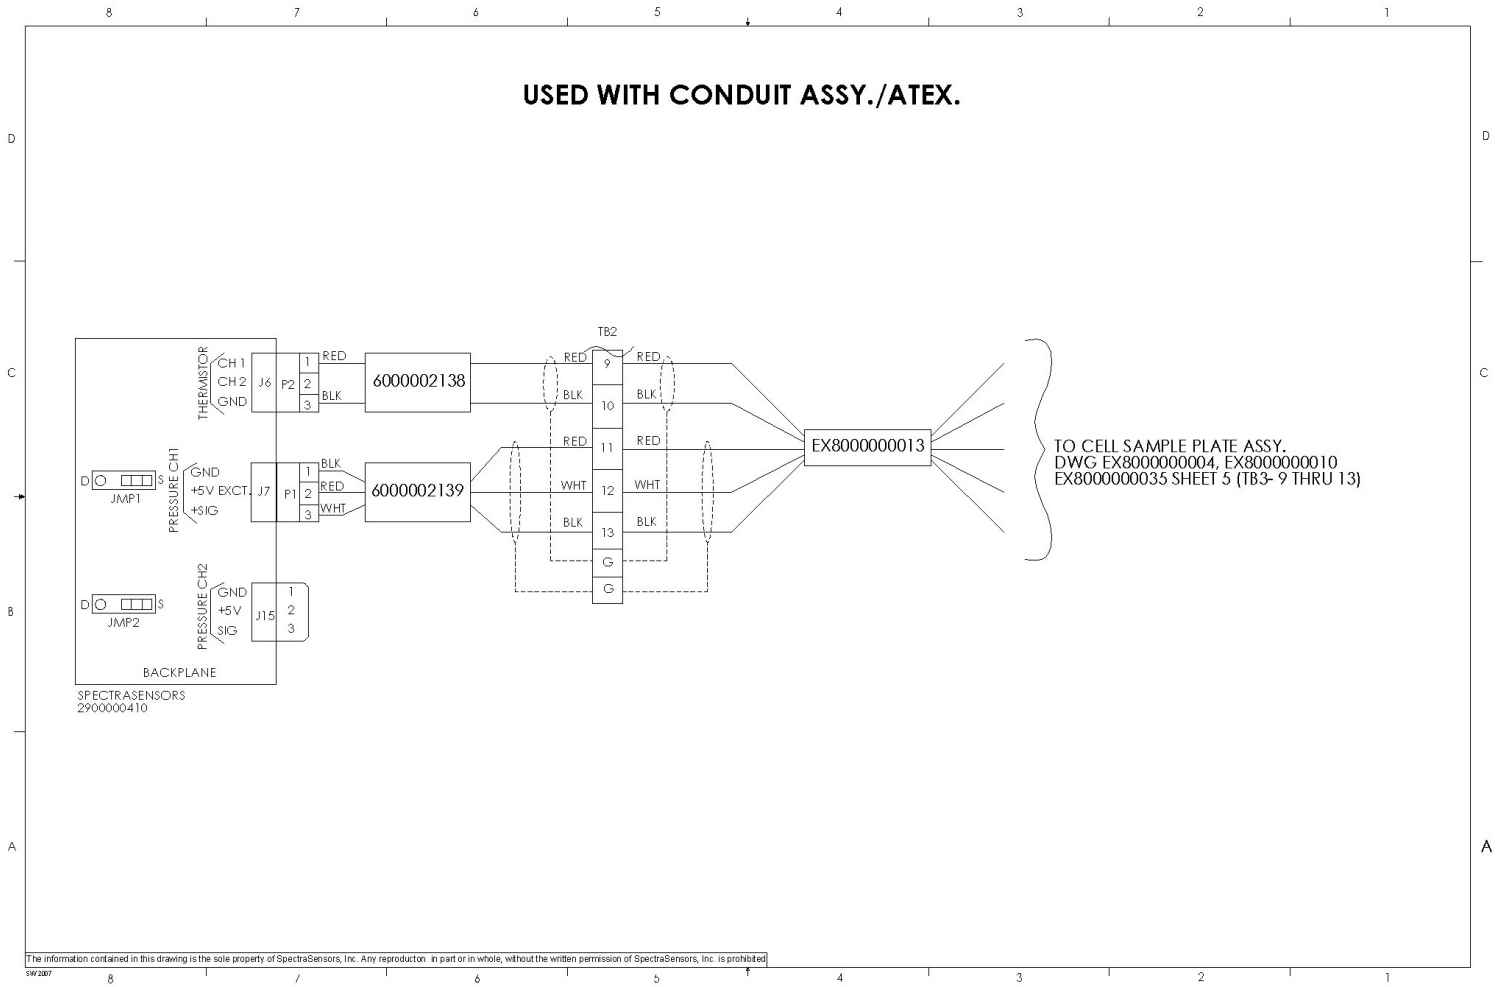


Figure D-8 Wiring schematic of conduit-coupled SS2100i-2 pressure and temperature sensor connections

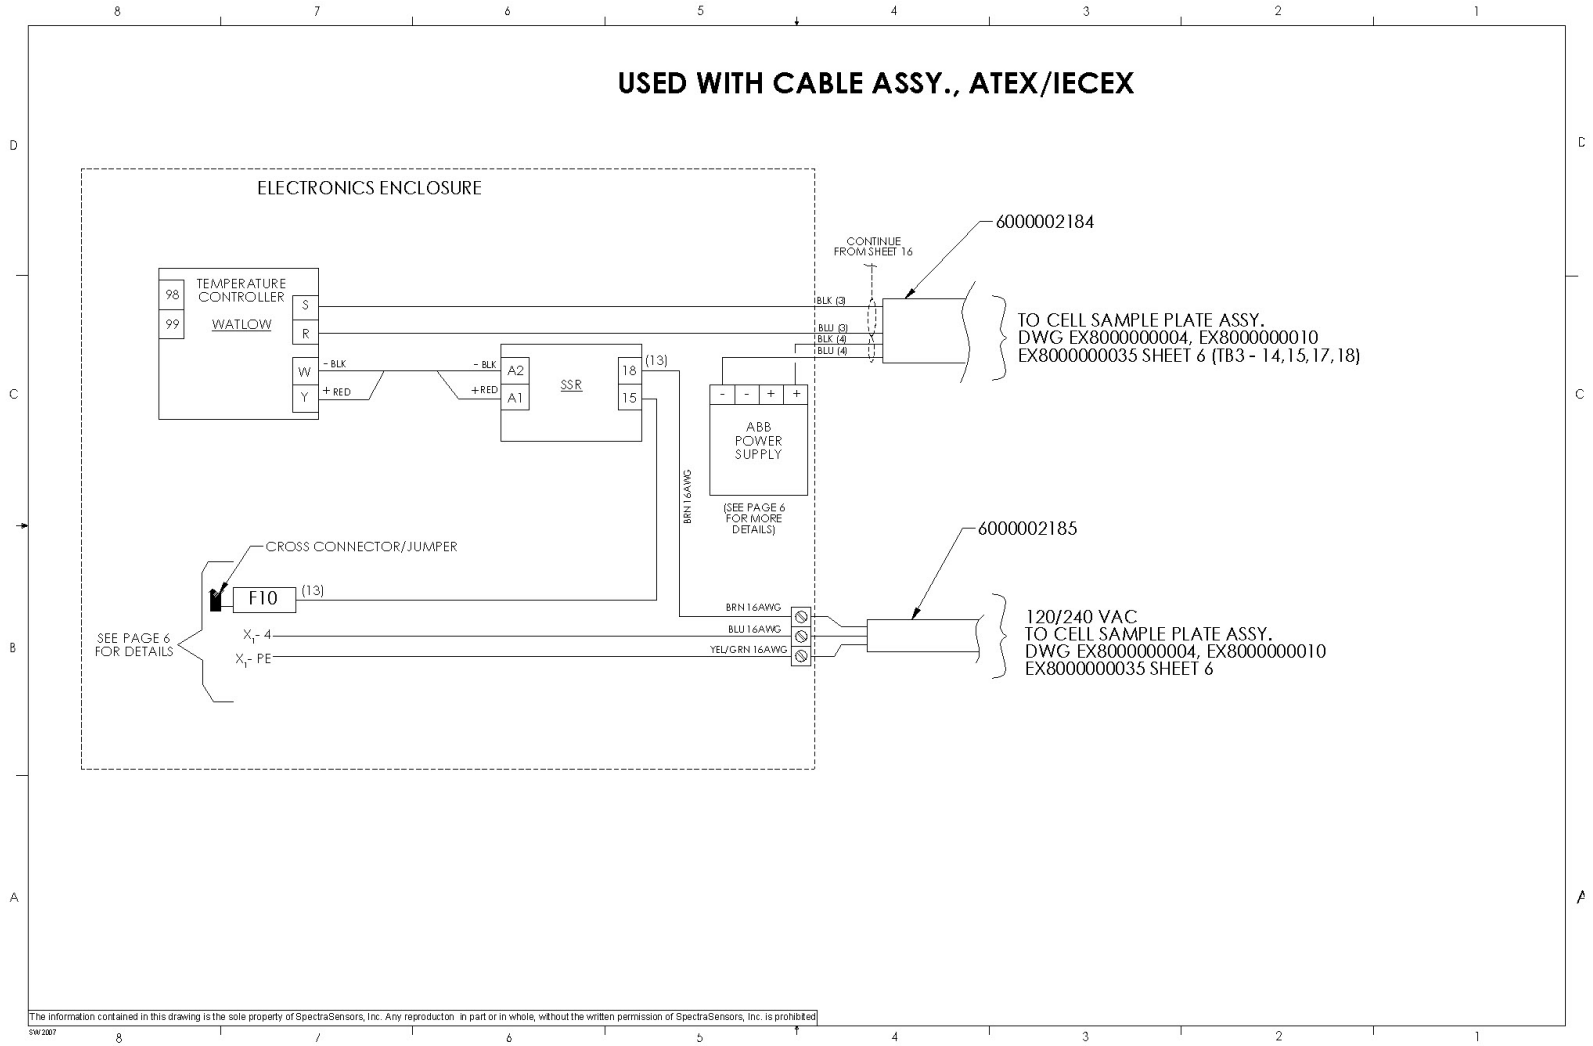


Figure D-9 Wiring schematic of cable-coupled SS2100i-2 power system

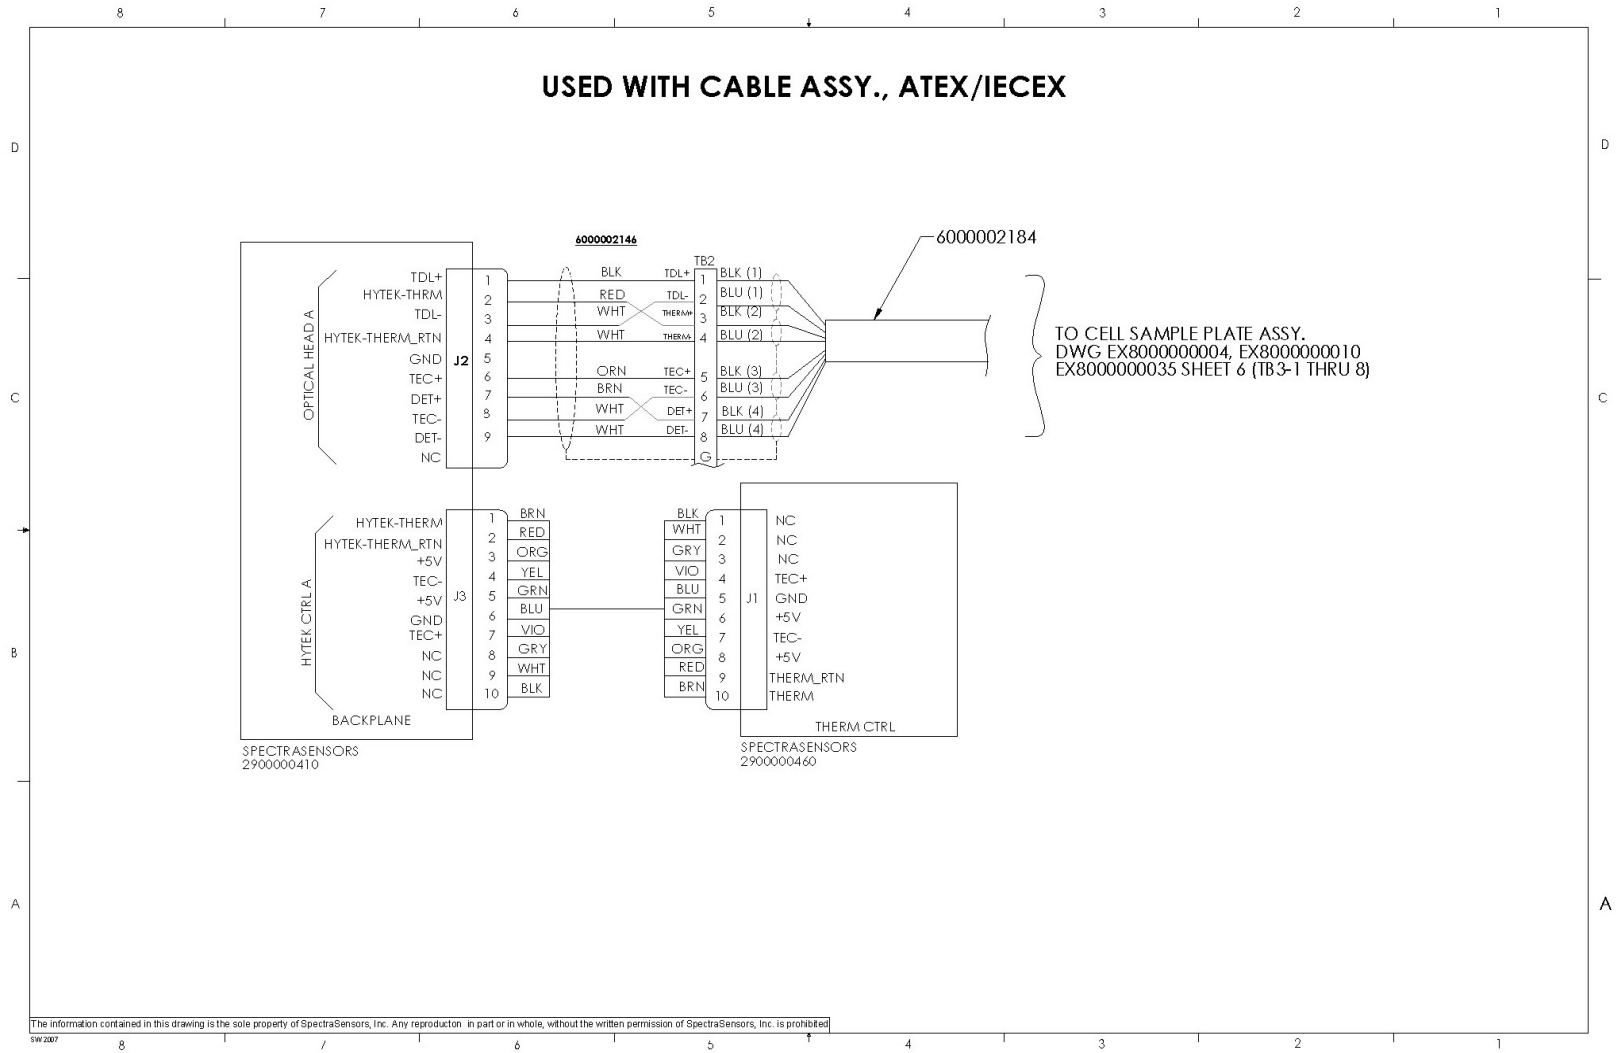


Figure D-10 Wiring schematic of cable-coupled SS2100i-2 optical head connections

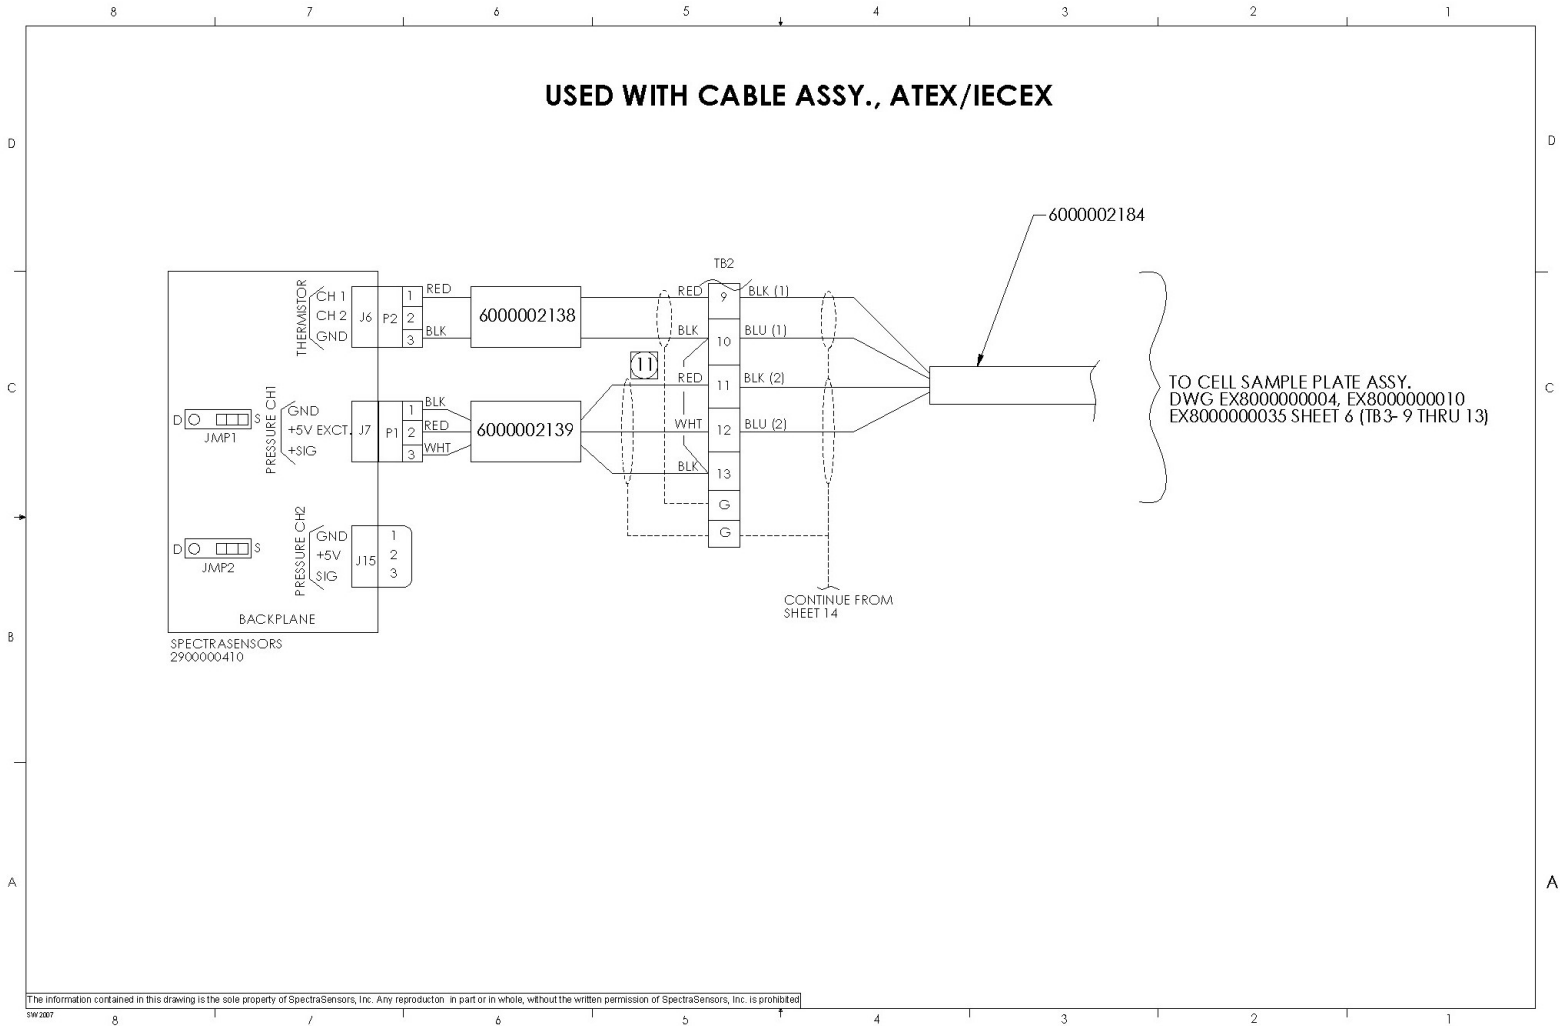


Figure D-11 Wiring schematic of cable-coupled SS2100i-2 pressure and temperature sensor connections

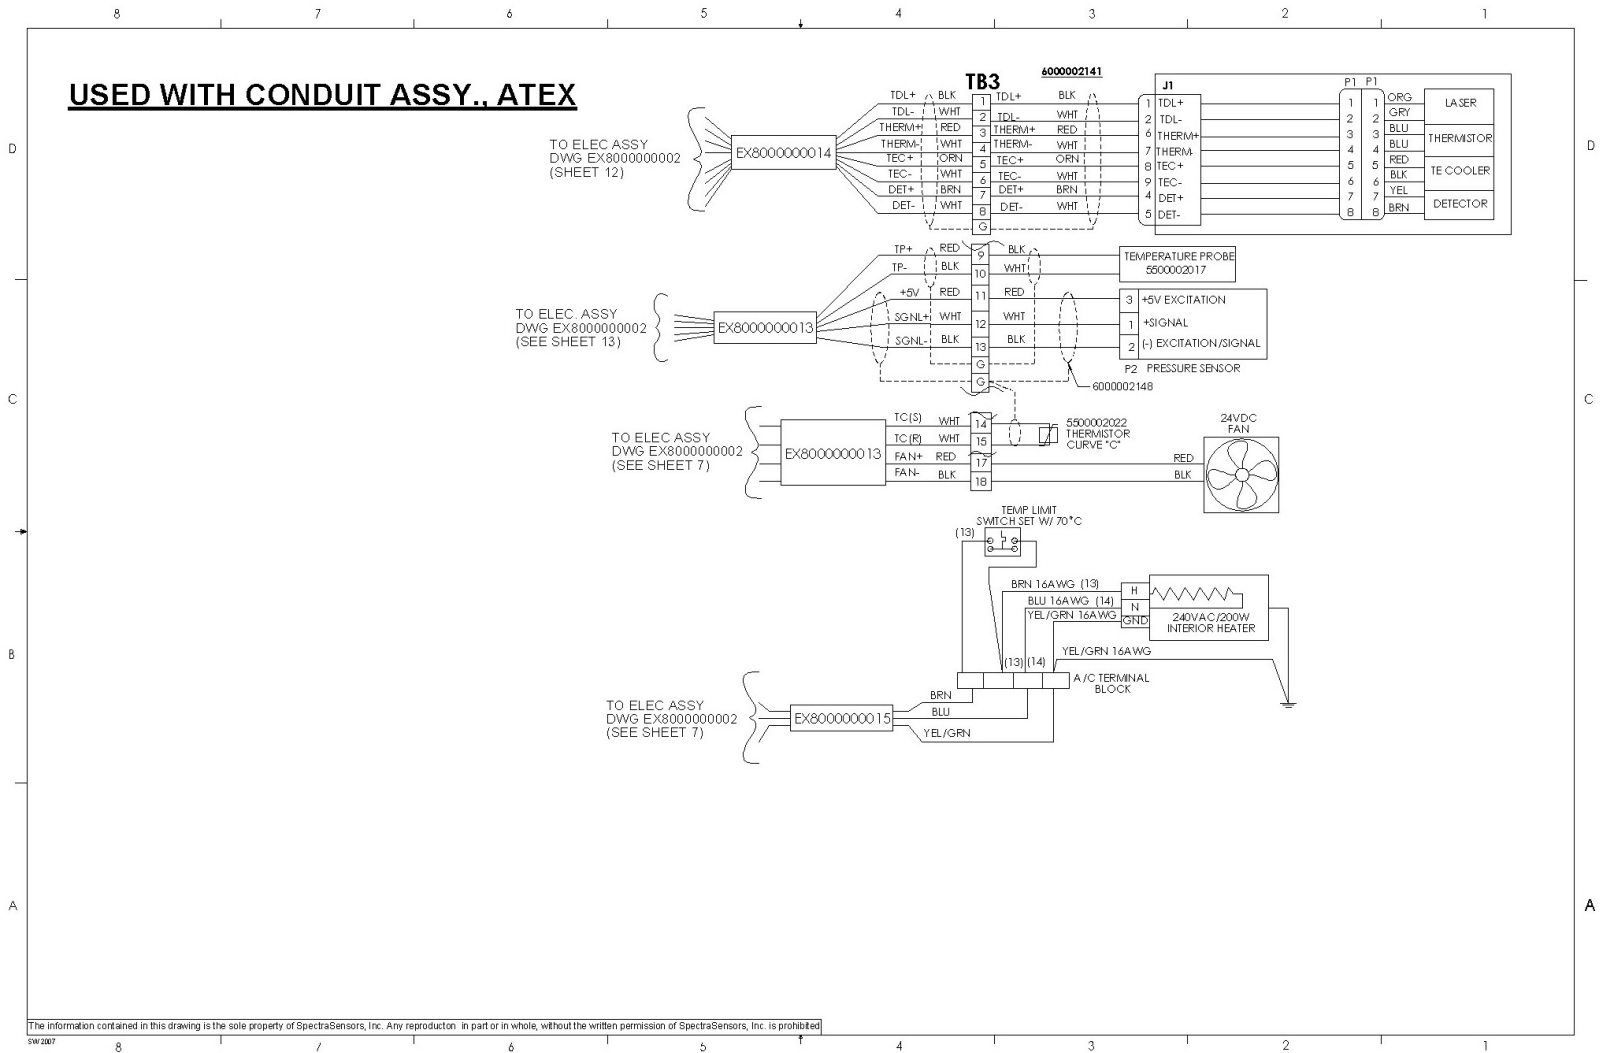


Figure D-12 Wiring schematic of conduit-coupled SS2100i-2 sample cell plate connections

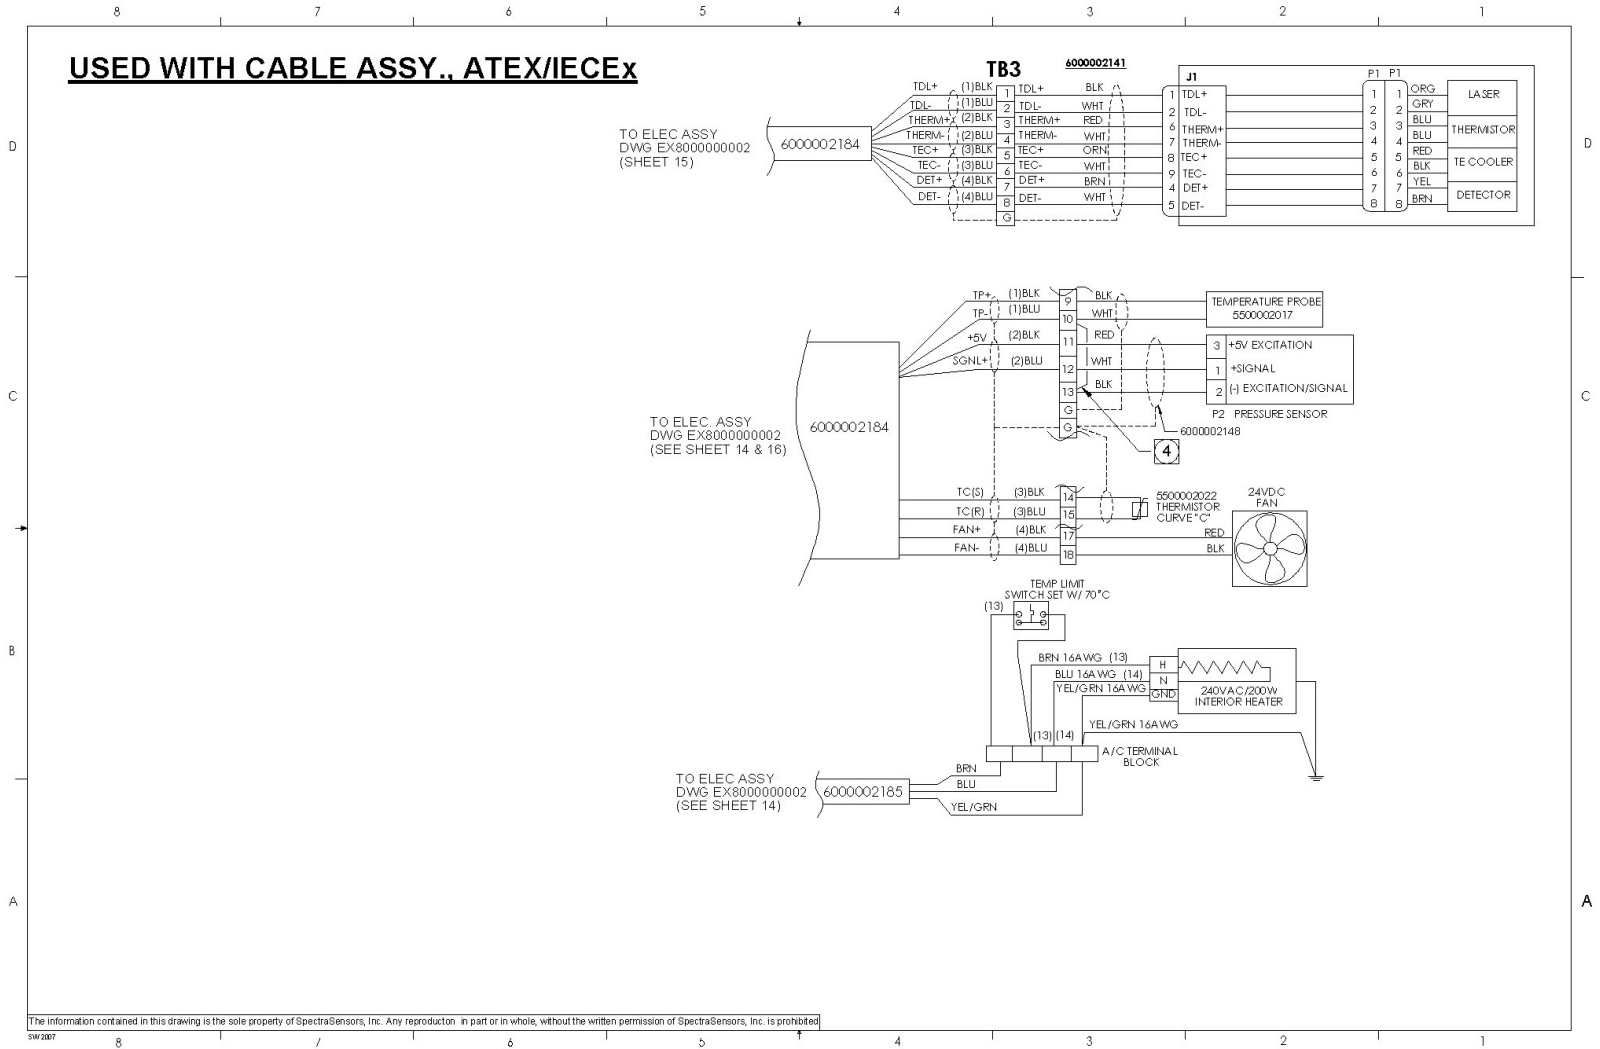


Figure D-13 Wiring schematic of cable-coupled SS2100i-2 sample cell plate connections

The information contained in this drawing is the sole property of SpectraSensors, Inc. Any reproduction, in part or in whole, without the written permission of SpectraSensors, Inc. is prohibited.

THIS PAGE INTENTIONALLY LEFT BLANK

BA02197C/66/EN/01.21

www.endress.com
